

743 Rancimat



Manual

8.743.8003EN / 2019-09-25



Metrohm AG

CH-9100 Herisau

Switzerland

Phone +41 71 353 85 85

Fax +41 71 353 89 01

info@metrohm.com

www.metrohm.com

743 Rancimat

Manual

Technical Communication
Metrohm AG
CH-9100 Herisau
techcom@metrohm.com

This documentation is protected by copyright. All rights reserved.

This documentation has been prepared with great care. However, errors can never be entirely ruled out. Please send comments regarding possible errors to the address above.

Table of contents

1	Introduction	1
1.1	Instrument description	1
1.2	Rancimat method	2
1.3	About the documentation	3
1.3.1	Symbols and conventions	3
1.4	Safety instructions	4
1.4.1	General notes on safety	4
1.4.2	Electrical safety	5
1.4.3	Flammable solvents and chemicals	6
1.4.4	Recycling and disposal	6
2	Overview of the instrument	7
3	Installation	10
3.1	Setting up the instrument	10
3.1.1	Packaging	10
3.1.2	Checks	10
3.1.3	Location	10
3.2	Mounting accessories	10
3.2.1	Mounting accessories for the internal air supply	10
3.2.2	Mounting accessories for the external air supply	13
3.2.3	Equipping the reaction and measuring vessels	13
3.2.4	Inserting vessels / Establishing tubing connections	16
3.2.5	Mounting the exhaust collection tube (optional accessories)	17
3.3	Mains connection	17
3.3.1	Checking the mains voltage	18
3.3.2	Replacing fuses	18
3.3.3	Connecting the instrument to the power grid	19
3.3.4	Switching the instrument on/off	19
3.4	Connecting a PC	20
3.4.1	Connecting the 743 Rancimat and the PC	20
3.4.2	Installing the software	20
3.4.3	Carrying out basic settings	22
4	Operation	25
4.1	Fundamentals of operation	25
4.1.1	Starting and exiting the program	25
4.1.2	Terms	26
4.1.3	Control window	26
4.1.4	Results window	28
4.1.5	File types	31
4.1.6	Context-sensitive menus	32



4.1.7	Mouse functions	32
4.1.8	Help	33
4.2	Instrument and Program Settings	34
4.2.1	Establishing the instrument communication	34
4.2.2	Managing access rights	35
4.2.3	Timer	38
4.2.4	Gas flow control	40
4.2.5	Recording the temperature	41
4.2.6	Optimizing program and database	42
4.3	Program information	43
4.3.1	Instrument information	43
4.3.2	Status overview	45
4.3.3	Displaying, filtering and deleting event overview	46
4.4	Calibration functions	49
4.4.1	Determining cell constants	49
4.4.2	Determining Delta T	51
4.5	Methods	56
4.5.1	Managing methods	56
4.5.2	Parameter description	61
4.6	Determinations	76
4.6.1	Preparing samples	77
4.6.2	Preparing the instrument and the accessories	80
4.6.3	Preparing the determination	82
4.6.4	Starting the determination	84
4.6.5	Cleaning the instrument and accessories	84
4.6.6	Adjusting the method parameters during the determination ..	85
4.6.7	Stopping the determination manually	86
4.6.8	Status of the live curve	87
4.7	Results	88
4.7.1	Determination overview	88
4.7.2	Determination and method data	104
4.7.3	Graph and reevaluation	113
4.7.4	Extrapolation	118
4.7.5	Recalculating a determination	122
4.7.6	Printing and exporting data	129
4.7.7	Program settings	136
4.7.8	Arranging windows	142
4.8	GLP functions	143
4.8.1	General information on GLP and validation	143
4.8.2	GLP monitoring	143
4.8.3	GLP status	145
4.8.4	Carrying out GLP tests	146
4.8.5	GLP results	156

5	Handling and maintenance	160
5.1	General information	160
5.1.1	Care	160
5.1.2	Maintenance by Metrohm Service	160
5.2	Replacing the dust filter	161
5.3	Regenerating or replacing the molecular sieve	161
5.4	Self test when switching on	162
6	Troubleshooting	163
6.1	Problems	163
7	Technical specifications	169
7.1	General data	169
7.2	Temperature regulation and measurement	169
7.3	Conductivity measurement	170
7.4	Gas flow regulation	170
7.5	GLP test set	171
7.6	RS-232 interface	171
7.7	Mains connection	171
7.8	Ambient temperature	172
7.9	Housing	172
8	Accessories	173
	Index	174



Table of figures

Figure 1	Measuring arrangement (schematic representation)	3
Figure 2	Front 743 Rancimat	7
Figure 3	Rear 743 Rancimat	8
Figure 4	Mounting accessories for the air supply (rear of the instrument)	11
Figure 5	Equipping the reaction and measuring vessels	14
Figure 6	Equipping the reaction vessel for determining Delta T	52
Figure 7	Accessories for GLP test Temperature	146

1 Introduction

1.1 Instrument description

The 743 Rancimat is a PC-controlled measuring device for determining the oxidation stability of samples containing oil and fat.

It is equipped with two **heating blocks** each with 4 measuring positions (channels). Every block can be heated individually, i.e. 4 samples can each be measured at 2 different temperatures or 8 samples at the same temperature. The measurements at the individual measuring positions can be started individually for this.

Operation of the 743 Rancimat is realized completely via a PC connected to the RS-232 interface using the control and evaluation program **743 Rancimat**. Up to 4 instruments can be connected to each PC, hence allowing a maximum of 32 samples to be analyzed. The evaluation algorithm of the PC program determines the break point of the Rancimat curve fully automatically and hence the induction time. Besides the **induction time**, the so-called **stability time**, i.e. the time duration until attaining a defined conductivity change, can also be determined. In the case of conductivity changes (stages) which do not have anything to do with the autoxidation, the evaluation can be interrupted for definite time intervals. The results determined can be processed further by computer. In particular, the induction times can be converted to the default temperatures of the corresponding standards.

Each Rancimat curve can also be evaluated **manually**. A PC-supported tangential method is available for this, in which you can position the tangents anywhere on your curves. This makes evaluations possible in extreme cases as well.

The results of the determinations are saved in a **database** together with all methods and determination data. Determinations can be searched for, sorted, filtered, exported and printed in the program part for the results display. Besides the graphic display of single and multiple curves, recalculation with altered parameters and extrapolation of the results to a definite temperature is also possible.

GLP (Good Laboratory Practice) and instrument validation are becoming increasingly important. The 743 Rancimat enables GLP tests for temperature, conductivity and gas flow measurement. You determine whether and which tests have to be carried out. You can also specify the time interval between the tests as well as the requirements regarding accuracy. If the GLP function has been selected, each result report will receive a comment



stating whether the GLP tests have been fulfilled. Metrohm offers a GLP test set to carry out these tests .

1.2 Rancimat method

The decay of vegetable and animal fats, which can be perceived in the initial stage through a deterioration of odor and taste (rancidity), is to a great extent the result of chemical alterations caused by the effect of atmospheric oxygen. These oxidation processes progressing slowly at ambient temperatures are referred to as **autoxidation**. They start with radical reactions on unsaturated fatty acids and undergo a process involving multiple stages resulting in diverse decomposition products, in particular peroxides as primary oxidation products and alcohols, aldehydes and carboxylic acids as secondary oxidation products.

With the **Rancimat method**, the sample is exposed to an air flow at a constant temperature between 50...220 °C (*see figure 1, page 3*). Highly volatile, secondary oxidation products (for the most part formic acid) are transferred into the measuring vessel with the air flow, where they are absorbed in the measuring solution (distilled water). Here the conductivity is continuously registered. The organic acids can thus be detected by increasing the conductivity. The time until occurrence of these secondary reaction products is referred to as the induction time or induction period, which is a good indicator for the oxidation stability.

The Rancimat method has been developed as an automated variant to the extremely complex AOM (active oxygen method) for determining the **induction time** of fats and oils. This method has become established over the course of time and has been incorporated in various national and international standards, e.g. AOCS Cd 12b-92 and ISO 6886.

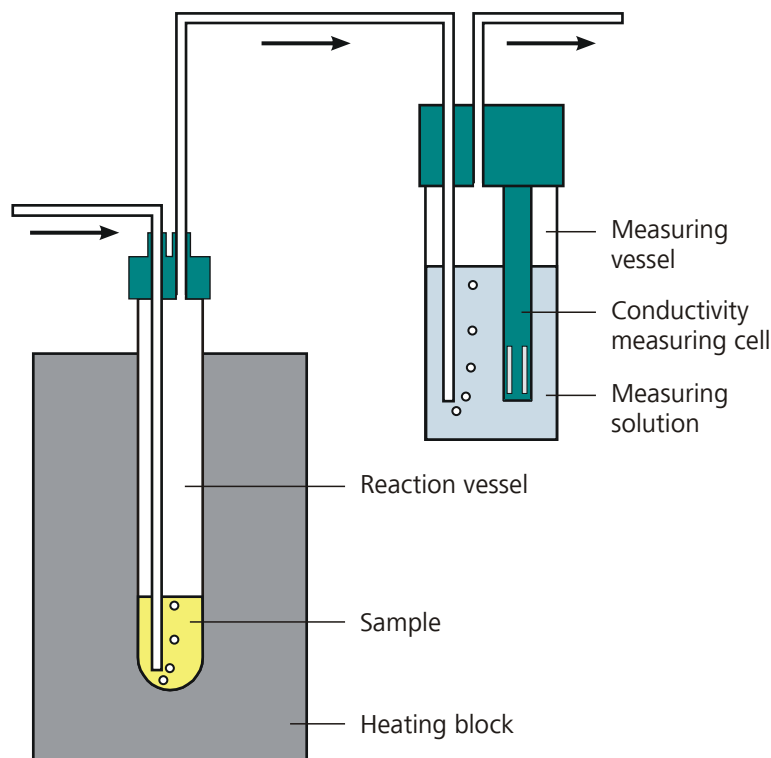


Figure 1 Measuring arrangement (schematic representation)

1.3 About the documentation



CAUTION







Please read through this documentation carefully before putting the instrument into operation. The documentation contains information and warnings which have to be followed by the user in order to ensure safe operation of the instrument.

1.3.1 Symbols and conventions

The following symbols and styles are used in this documentation:

(5-12)	Cross-reference to figure legend The first number refers to the figure number, the second to the instrument part in the figure.
1	Instruction step Carry out these steps in the sequence shown.
Method	Dialog text, parameter in the software
File ► New	Menu or menu item



[Next]	Button or key
	Warning This symbol draws attention to a possible life hazard or risk of injury.
	Warning This symbol draws attention to a possible hazard due to electrical current.
	Warning This symbol draws attention to a possible hazard due to heat or hot instrument parts.
	Warning This symbol draws attention to a possible biological hazard.
	Caution This symbol draws attention to a possible damage of instruments or instrument parts.
	Note This symbol marks additional information and tips.

1.4 Safety instructions

1.4.1 General notes on safety



WARNING

Operate this instrument only according to the information contained in this documentation.

This instrument has left the factory in a flawless state in terms of technical safety. To maintain this state and ensure non-hazardous operation of the instrument, the following instructions must be observed carefully.

Hot reaction vessels



WARNING

The reaction vessels can become very hot.

Avoid any contact with the hot reaction vessels. Place these in the vessel holders provided for cooling down.

Flammable substances



WARNING

The heating block of the 743 Rancimat can be heated to 229.9 °C.

Flammable substances may ignite at such temperatures.

Adjust the oven's maximum heating temperature to the sample that is to be analyzed.

Defective glass vessels



WARNING

Caution with defective glass vessels.

An overflow of flammable samples into the heating block can be dangerous.

Check the glass vessels before each use.

1.4.2 Electrical safety

The electrical safety when working with the instrument is ensured as part of the regulations IEC 1010-1 (protection class 1, degree of protection IP20).



WARNING

Only personnel qualified by Metrohm are authorized to carry out service work on electronic components.



WARNING

Never open the housing of the instrument. The instrument could be damaged by this. There is also a risk of serious injury if live components are touched.

There are no parts inside the housing which can be serviced or replaced by the user.



Mains voltage



WARNING

An incorrect supply voltage can damage the instrument.

Only operate this instrument with a supply voltage specified for it (see rear panel of the instrument).

Protection against electrostatic charges



WARNING

Electronic components are sensitive to electrostatic charges and can be destroyed by discharges.

Do not fail to pull the power cord out of the power socket before you set up or disconnect electrical plug connections at the rear of the instrument.

1.4.3 Flammable solvents and chemicals




WARNING

All relevant safety measures are to be observed when working with flammable solvents and chemicals.

- Set up the instrument in a well-ventilated location (e.g. fume cupboard).
- Keep all sources of flame far from the workplace.
- Clean up spilled liquids and solids immediately.
- Follow the safety instructions of the chemical manufacturer.

1.4.4 Recycling and disposal



This product is covered by European Directive 2012/19/EU, WEEE – Waste Electrical and Electronic Equipment.

The correct disposal of your old instrument will help to prevent negative effects on the environment and public health.

More details about the disposal of your old instrument can be obtained from your local authorities, from waste disposal companies or from your local dealer.

2 Overview of the instrument

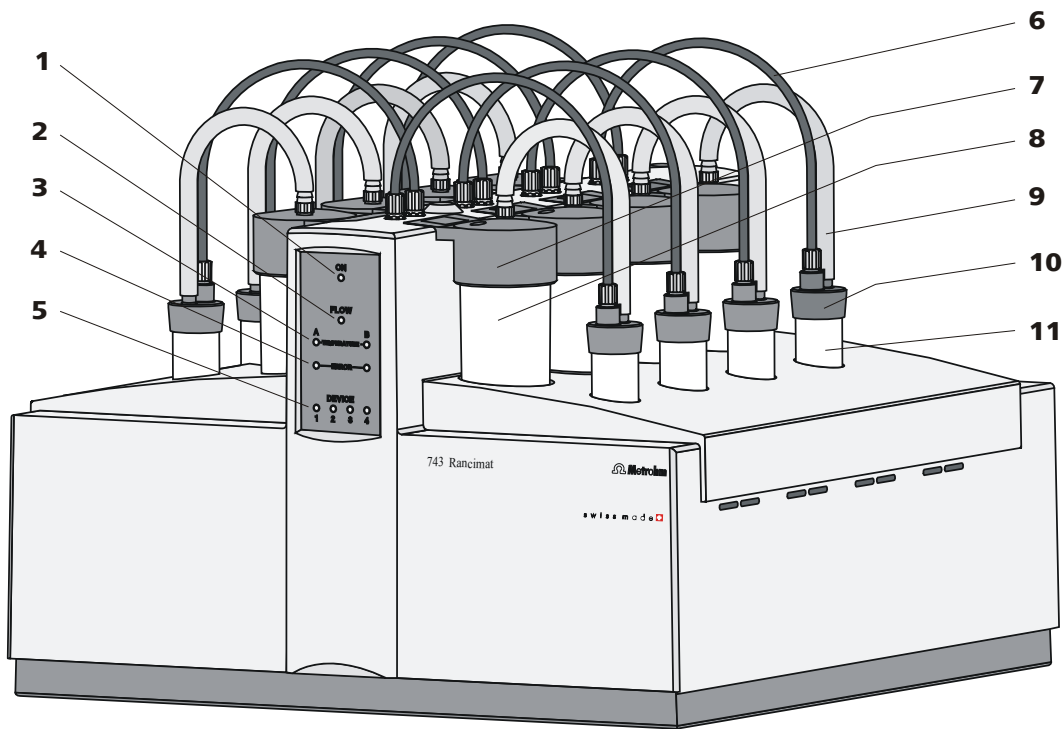


Figure 2 Front 743 Rancimat

1 Pilot lamp

Lights up when the instrument is switched on.

3 Temperature display

Flashes when the heating is switched on.
Lights up when the temperature has been reached.

5 Instrument number display

Indicates the number of the instrument.
Lights up if the instrument is registered.
Flashes (all LEDs) if the connection to the PC is interrupted.

7 Measuring vessel cover (6.0913.130)

Contains an integrated conductivity measuring cell.

2 Gas flow display

Flashes when the gas flow is switched on.
Lights up when the gas flow has been reached.

4 Error display (red)

Lights up or flashes when a fault has occurred in the instrument (see *Troubleshooting Chapter*).

6 FEP tubing 250 mm (6.1805.080)

For supplying air into the reaction vessel.

8 Measuring vessel (6.1428.100)



9 Silicone tubing (6.1816.010)
For connecting the reaction vessel to the measuring vessel.

10 Reaction vessel cover (6.2753.107)

11 Reaction vessel (6.1429.040)

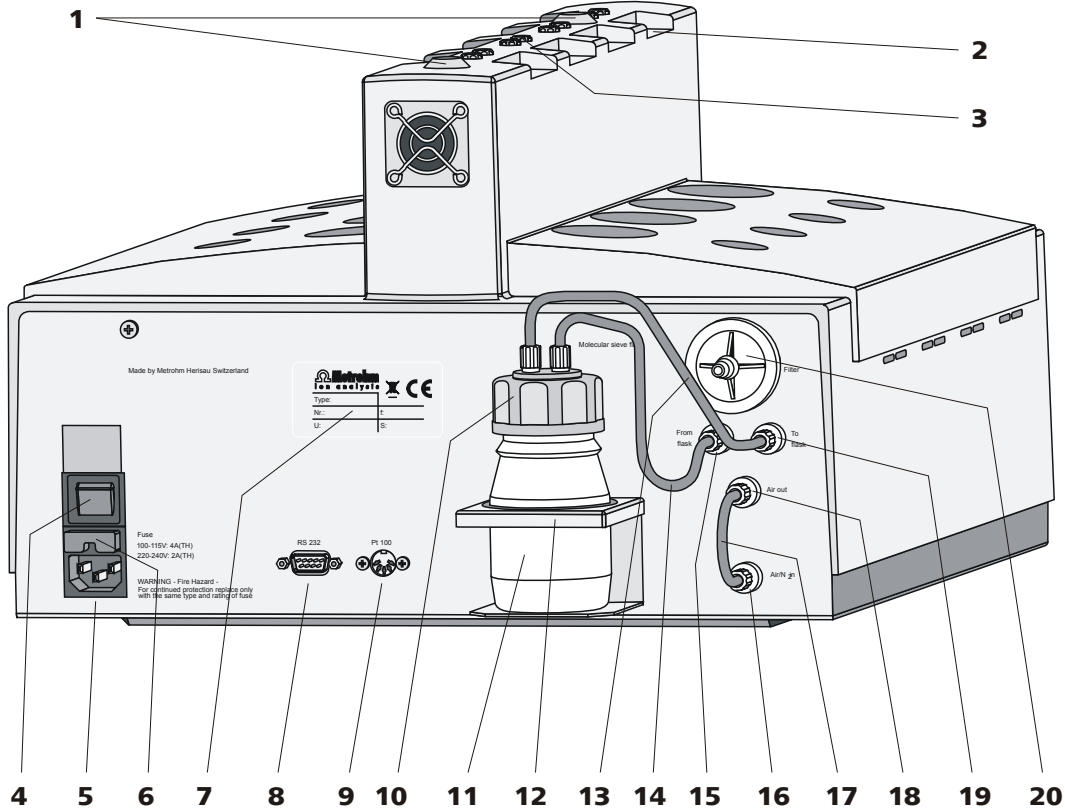


Figure 3 Rear 743 Rancimat

1 Collection tube holder
For fastening the optional exhaust collection tube (6.2757.000).

2 Electrode connector
For connecting the conductivity measuring cell integrated in the measuring vessel cover (2-7).

3 Air supply connection
For connecting the FEP tubing 250 mm (2-6).

4 Mains switch
For turning the instrument on and off.
I = ON / 0 = OFF.

5 Mains connection socket
For important information on the mains connection, see Chapter 3.3.

6 Fuse holder
Replacing fuses, see Chapter 3.3.2.

7 Type plate
Contains specifications concerning mains voltage and serial number.

8 RS-232 connector
For connecting the PC.

9 Pt100 connector For connecting an external temperature sensor.	10 Drying flask cover (6.1602.145) Cover for the drying flask.
11 Drying flask (6.1608.050)	12 Flask holder For fastening the drying flask.
13 FEP tubing 250 mm (6.1805.080) For supplying the air from the internal pump to the drying flask.	14 FEP tubing 250 mm (6.1805.080) For supplying the air from the drying flask to the reaction vessel (2- 11).
15 "From Flask" connection	16 "Air/N₂ in" connection
17 FEP tubing 130 mm (6.1805.010) For connecting the Air out connection to the Air/N₂ in connection during normal operation with the internal air pump.	18 "Air out" connection
19 "To Flask" connection	20 Dust filter (6.2724.010)



3 Installation

3.1 Setting up the instrument

3.1.1 Packaging

The instrument is supplied in protective packaging together with the separately packed accessories. Keep this packaging, as only this ensures safe transportation of the instrument.

3.1.2 Checks

Immediately after receipt, check whether the shipment has arrived complete and without damage by comparing it with the delivery note.

3.1.3 Location

The instrument has been developed for operation indoors and may not be used in explosive environments.

Place the instrument in a location of the laboratory suitable for operation and free of vibrations, if possible protected from corrosive atmospheres and contamination by chemicals.

The instrument should be protected against excessive temperature fluctuations and direct sunlight.



NOTICE

In order to improve accessibility for the measuring positions, the instrument can be placed on the optionally available 6.2059.000 turning ring.

3.2 Mounting accessories

3.2.1 Mounting accessories for the internal air supply

The gas in the Rancimat is normally supplied using the **internal air pump**, which sucks in **laboratory air**. For air supply and air purification, the following accessories must be mounted on the rear of the Rancimat:

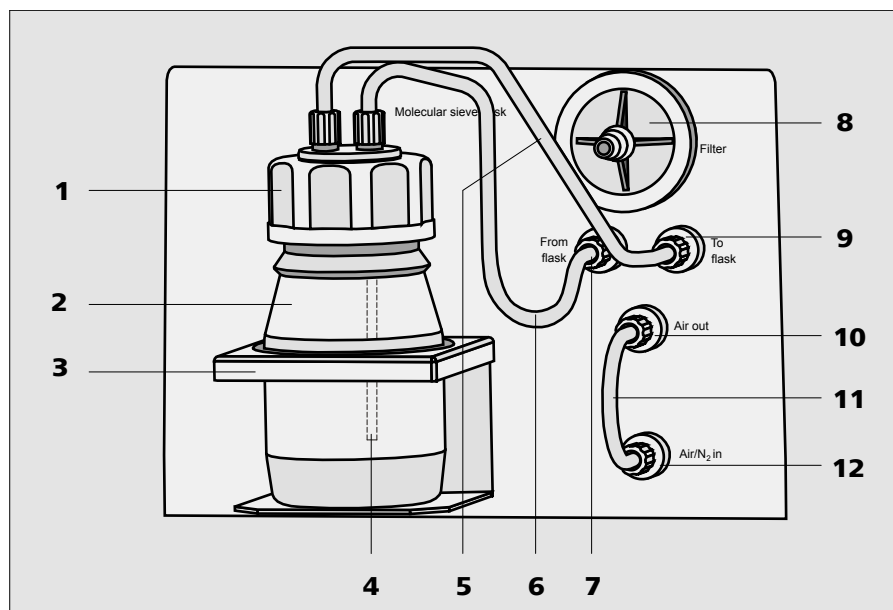


Figure 4 Mounting accessories for the air supply (rear of the instrument)

1 Drying flask cover (6.1602.145) Cover for the drying flask.	2 Drying flask (6.1608.050)
3 Flask holder For fastening the drying flask.	4 Filter tube (6.1821.040)
5 FEP tubing 250 mm (6.1805.080) For supplying the air from the internal pump to the drying flask.	6 FEP tubing 250 mm (6.1805.080) For supplying the air from the drying flask to the reaction vessel (2- 11).
7 "From Flask" connection	8 Dust filter (6.2724.010)
9 "To Flask" connection	10 "Air out" connection
11 FEP tubing 130 mm (6.1805.010)	12 "Air/N₂ in" connection

Mount the accessories for the air supply as follows:

1 Mount dust filter

- Insert the dust filter (4-8) on the connection marked with **Filter** on the rear of the Rancimat.
- If the laboratory air is heavily contaminated, a tubing for supplying fresh air can be connected to the dust filter.

**NOTICE**

The dust filter serves for filtering the air sucked through the air pump and must be replaced at periodic intervals (*see chapter 5.2, page 161*).

2 Mount drying flask**CAUTION**

Do **not** fill the hot molecular sieve directly into the drying flask after regeneration, as otherwise the plastic filter on the filter tube will melt.

Wait until the molecular sieve has cooled down before filling.

- Fill the molecular sieve into the drying flask (4-2).
- Screw the filter tube (4-4) on the lower side of the drying flask cover (4-1) into the opening marked (above) with a dot.
- Screw the drying flask cover with mounted filter tube onto the drying flask and insert in the flask holder (4-3) on the rear of the Rancimat.
- Screw the one end of the FEP tubing 250 mm (4-6) onto that opening on the drying flask cover at the bottom of which the filter tube is located.
- Screw the other end of the FEP tubing onto the **From flask** connection (4-7) on the rear of the Rancimat.
- Screw the one end of the second FEP tubing 250 mm (4-5) onto the second opening on the drying flask cover.
- Screw the other end of the second FEP tubing onto the **To flask** connection (4-9).

**NOTICE**

The molecular sieve serves for adsorbing interfering oxidizing gases as well as water from the sucked in air. You can regenerate it in the drying oven at +140...+180 °C for 24 to 48 h (*see chapter 5.3, page 161*).

3 Mount the FEP tubing for the supply air

- Screw the one end of the FEP tubing 130 mm (4-11) onto the **Air out** connection (4-10).

- Screw the other end of the FEP tubing onto the **Air/N₂ in** connection (4-12).

3.2.2 Mounting accessories for the external air supply

If the laboratory air is heavily contaminated, an external gas supply with synthetic air can be provided. For this, the corresponding accessories must be mounted on the rear of the Rancimat.

Mount the accessories for the external air supply as follows:

1 Mount the FEP tubing

- Screw the one end of the FEP tubing 130 mm (4-11) onto the **Air/N₂ in** connection (4-12) on the rear of the Rancimat.
- Screw the tubing adapter M6 / olive (6.1808.020) onto the other end of the FEP tubing.

2 Connect the gas supply

- Mount the gas supply from the bomb with synthetic air onto the tubing adapter M6 / olive (6.1808.020).



NOTICE

With an external gas supply, the gas flow cannot be regulated in the PC program. The gas flow must be set manually using the reducing valve and the gas flow display (see chapter 4.2.4, page 40).

3.2.3 Equipping the reaction and measuring vessels

The following figure shows in detail, how the accessories parts for measuring the oxidation stability have to be mounted and connected to one another.

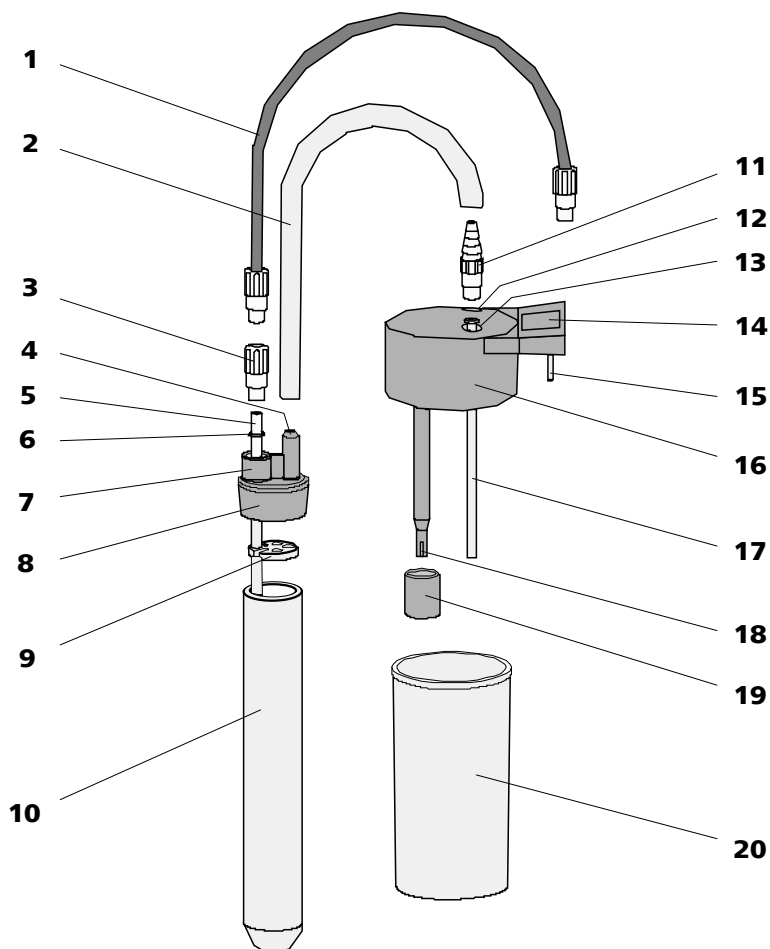


Figure 5 Equipping the reaction and measuring vessels

1	FEP tubing 250 mm (6.1805.080) For supplying air into the reaction vessel.	2	Silicone tubing (6.1816.010) For connecting the reaction vessel to the measuring vessel.
3	Thread adapter M8 / M6 (6.1808.090)	4	Tubing connector For connecting the silicone tubing.
5	Air tube (6.2418.100)	6	O-ring (6.1454.040)
7	Connection For connecting the thread adapter M8 / M6.	8	Reaction vessel cover (6.2753.107)
9	Foam barrier (6.1451.010)	10	Reaction vessel (6.1429.040)
11	Tubing adapter M8 / olive (6.1808.050) For connecting the silicone tubing to the opening In (5-13).	12	Opening "Out" For removing the air from the measuring vessel.
13	Opening "In" For supplying the air to the measuring vessel.	14	Labeling field For entering the cell constant.

15 Connector plug	16 Measuring vessel cover (6.0913.130) Contains integrated conductivity measuring cell.
17 PTFE tube (6.1819.080) For supplying the air to the measuring solution.	18 Electrode
19 Protection ring	20 Measuring vessel (6.1428.100)

Proceed as follows to mount the measuring and reaction vessel:

1 Mount the measuring vessel cover

- Insert the PTFE tube (5-17) from above into the opening **In** (5-13) of the measuring vessel cover.
- Screw the tubing adapter M8 / olive (5-11) into the opening **In** of the measuring vessel cover.
- Place the measuring vessel cover (5-16) on the measuring vessel (5-20).

2 Mount the reaction vessel cover

- Insert the air tube (5-5) from below into the connection (5-7) of the reaction vessel cover.
- Place the O-ring (5-6) over the upper end of the air tube.
- Screw the thread adapter M8 / M6 (5-3) gently into the connection (5-7) and, at the same time, press the air tube against the thread adapter M8 / M6.
- Now fix the air tube onto the reaction vessel cover by firmly pulling the thread adapter M8 / M6.
- If determinations are carried out with highly foaming samples, clamp the foam barrier (5-9) onto the air tube.
- Place the reaction vessel cover on the reaction vessel.



WARNING

The foam barrier can melt if it projects too deeply into the heating block.

Ensure that the foam barrier is **at least 7 cm** above the base of the reaction vessel.



3.2.4 Inserting vessels / Establishing tubing connections

After you have assembled the reaction and measuring vessels, insert them in the Rancimat and establish the tubing connections as follows:

1 Insert the measuring vessel

- Fill the measuring vessel (5-20) with distilled water.
- Place the measuring vessel cover on the measuring vessel.
- Insert the measuring vessel into the openings provided on the Rancimat. At the same time, carefully insert the connector plugs (5-15) into the electrode connector (3-2).
- Connect the white silicon tubing (5-2) to the tubing adapter M8 / olive (5-11) of the measuring vessel cover.

2 Mount the tubings for the air supply

- Screw the FEP tubings 250 mm onto the air supply connections (3-3) of the Rancimat.

3 Insert the reaction vessel

- Fill the reaction vessel (5-10) with the sample.
- After reaching the required temperature, insert the reaction vessel with the mounted reaction vessel cover in the openings provided on the Rancimat.

4 Establish the tubing connections

- Connect the white silicone tubing (5-2), which is fastened on the measuring vessel cover, to the tubing connector (5-4) of the reaction vessel cover.
- Screw the FEP tubing 250 mm (5-1), which is fastened on the tubing adapter M8 / olive (5-11) of the Rancimat, onto the thread adapter M8 / M6 (5-3) of the reaction vessel cover.



NOTICE

Instead of the measuring vessel 6.1428.100 made from polycarbonate, the optionally available measuring vessel 6.1428.020 made from clear glass can be used. In contrast to the polycarbonate vessel, the measuring vessel 6.1428.020 can also be cleaned with acetone.

3.2.5 Mounting the exhaust collection tube (optional accessories)

The optionally available exhaust collection tube 6.2757.000 can be mounted on the 743 Rancimat for targeted removal of the exhaust air. In addition to the exhaust collection tube, 8 silicone tubings 6.1816.010 (220 mm) also have to be ordered.

Proceed as follows to mount the collection tube:

1 Mount the exhaust collection tube

- Insert the exhaust collection tube with both nozzles into the collection tube holders (3-1) on the Rancimat in such a way that the connection to the exhaust air removal is located to the rear.

2 Connect the measuring vessels

- Screw the tubing adapter M8 / olive (5-11) into the opening **Out** (5-12) of the measuring vessel cover.
- Connect the one end of the silicone tubing (5-2) to the tubing adapter M8 / olive.
- Insert the other end of the silicone tubing into the corresponding opening on the collection tube.
- Seal the unused openings on the collection tube with the enclosed plugs E.400.0010.

3 Connect the exhaust collection tube

- Connect a suitable tubing to the connection of the exhaust collection tube and connect this to an active suction device (e.g. water jet pump).

3.3 Mains connection



WARNING

There is a risk of fire if the instrument is operated with an incorrect mains fuse!

Follow the regulations below for the mains connection.



3.3.1 Checking the mains voltage

Before switching the 743 Rancimat on for the first time, check whether the mains voltage indicated on the type plate (3-7) corresponds to the mains voltage present. If this is not the case, please contact Metrohm Service.

3.3.2 Replacing fuses

Two fuses 4 A (slow-acting) for 115 V or 2 A (slow-acting) for 230 V are installed in the fuse holder (3-6) of the 743 Rancimat as standard.



WARNING

Ensure that the instrument is never put into operation with fuses of another type, otherwise there is a risk of fire!

Proceed as follows to replace defective fuses:

1 Pull out the mains cable

- Pull the mains cable out of the mains connection socket of the Rancimat.

2 Remove the fuse holder

- Use a screwdriver to loosen and completely pull out the fuse holder (3-6) above the mains connection socket.

3 Replace fuses

- Carefully take the defective fuses out of the fuse holder and replace them with two new fuses suitable for the set mains voltage of the type TH (slow-acting, with high switching capacity):
 - 115 V 4 A (TH) Metrohm No.: U.600.0022
 - 230 V 2 A (TH) Metrohm No. U.600.0107

4 Insert the fuse holder

- Push the fuse holder back into the instrument until it latches into place.

3.3.3 Connecting the instrument to the power grid



WARNING

Electric shock from electrical potential

Risk of injury by touching live components or through moisture on live parts.

- Never open the housing of the instrument while the power cord is still connected.
- Protect live parts (e.g. power supply unit, power cord, connection sockets) against moisture.
- Unplug the power plug immediately if you suspect that moisture has gotten inside the instrument.
- Only personnel who have been issued Metrohm qualifications may perform service and repair work on electrical and electronic parts.

Connecting the power cord

Accessories

Power cord with the following specifications:

- Length: max. 2 m
- Number of cores: 3, with protective conductor
- Instrument plug: IEC 60320 type C13
- Conductor cross-section 3x min. 0.75 mm² / 18 AWG
- Power plug:
 - according to customer requirement (6.2122.XX0)
 - min. 10 A



NOTICE

Do not use a not permitted power cord!

1 Plugging in the power cord

- Plug the power cord into the instrument's power socket.
- Connect the power cord to the power grid.

3.3.4 Switching the instrument on/off

The Rancimat is switched on and off using the mains switch. When switching the instrument on, the pilot lamp **ON** lights up on the front of the instrument.



3.4 Connecting a PC

3.4.1 Connecting the 743 Rancimat and the PC



CAUTION

Always switch the Rancimat and PC off before you connect the two devices with the RS-232 cable 6.2134.100.

The PC program **743 Rancimat** allows control of max. 4 instruments. The following options are available for connecting the instruments to serial PC interfaces:

- Connection to integrated COM interfaces of the PC
- Connection to an additional integrated interface expansion card

Connect the RS-232 interface of the Rancimat to the required serial COM port on the PC using the RS-232 cable 6.2134.100 (9-pin/9-pin). For 25-pin COM ports, the optional RS-232 cable 6.2125.110 (not in the scope of delivery) or a commercially available adapter must be used.

3.4.2 Installing the software

3.4.2.1 System requirements

Operating system	Windows 2000, Windows XP Professional, Windows Vista
RAM	256 MB (Windows 2000 / Windows XP) 1 GB (Windows Vista)
Processor	Pentium III or higher
Memory	approx. 20 MB for program files
RS-232 interface	one free RS-232 interface (COM)

The windows user must have administrator rights in order to be able to install 743 Rancimat.

3.4.2.2 Installing the program

Proceed as follows to install 743 Rancimat:

1 Start the installation program

- Place the installation CD in the CD drive. The installation program is started automatically.
If this option is deactivated on your computer, double click the file **Setup.exe**.
Windows Vista: Select the option "Approve".
- Click on **743**.

2 Select the dialog language

- Select the dialog language of the program.
- Click on the **[OK]** button.
- Click on the **[Next >]** button.

3 Accept the license agreement

- Read through the license agreement and accept it with **[Yes]**.

4 Define a target folder for the program

- If required, choose another folder than the default target folder for the program files. For that, click on the **[Browse...]** button.
- Confirm the target folder with **[Next >]**.

5 Define the components of the program

- Click on the **[Next >]** button.

6 Define a target folder for the program icon

- Choose or enter the program folder of the Start menu in which the program icon is to be inserted and confirm with **[Next >]**.

The program will be installed.

7 Complete the installation

- Click on the **[Finish]** button after the successfully completed installation.

The installation program will be exited.



3.4.2.3 Windows Vista



CAUTION

If you run the software 743 Rancimat on a computer with Windows Vista, you need a special update in order to be able to display the help. Due to licensing reasons you have to download this file from a Microsoft web page. On the installation CD the link "**Download Win-Help.url**" to the corresponding Microsoft web page can be found in the folder "**Vista Update for HLP help**". Download the necessary installation file and save it.

Proceed as follows to install the update:

- 1
 - Exit 743 Rancimat if you have started the software after the installation.
 - Start the installation file by double-clicking and follow the instructions of the installation program.


3.4.3 Carrying out basic settings

Setting the Administrator password

When starting the program for the first time, the Administrator password must be set. Proceed as follows:

- 1 **Switch on the instruments**
 - Check whether the Rancimat is correctly connected to the PC (*see chapter 3.4.1, page 20*).
 - Switch on the Rancimat using the mains switch.
 - Switch on the PC.
- 2 **Start program**
 - In the Windows Start menu under **Programs ▶ Metrohm ▶ Rancimat**, click on the menu item **Rancimat**.

The login window for the Administrator opens:

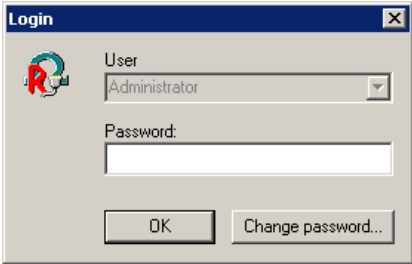


3 Set Administrator password

- Do **not** enter a password, instead click on **[OK]**.
- Confirm the displayed message with **[OK]**.
The following dialog window appears:



- Leave the **Old password** field empty.
- Enter a new password for the Administrator in the **New password** field.
- Reenter the password in the **Confirm new password** field and confirm with **[OK]**.

The dialog window **Login** opens again:

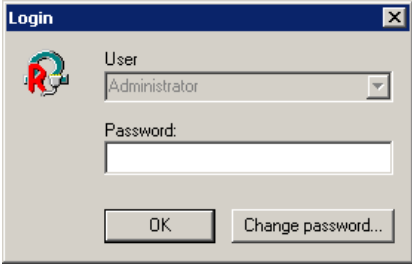

4 Log in as Administrator

- Enter the Administrator password set before in the **Password** field and confirm with **[OK]**.
- Confirm the message **"There are no units configured yet!"** with **[OK]**.



Establishing the device communication

- 1 Follow the instructions in Section 4.2.1.

4 Operation

This section describes the most important points for operation of the 743 Rancimat.

You can find more detailed information in the Online help of the software, which you can use to rapidly and easily call up the required information everywhere, via **[F1]**.

4.1 Fundamentals of operation

4.1.1 Starting and exiting the program

Proceed as follows to start and exit the program:




NOTICE

If you are starting the program for the first time, you first have to set an Administrator password (see chapter 3.4.3, page 22).

1 Start program

- In the Windows Start menu under **Programs ▶ Metrohm ▶ Rancimat**, click on the menu item **Rancimat**.

The following dialog window appears:

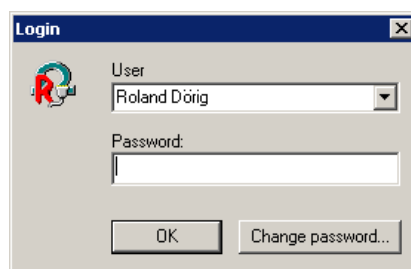

2 Log in

- Select the required **User**.
- Enter the **Password** and confirm with **[OK]**.

3 Close program

- Click on the menu item **File ▶ Exit** or the symbol **✕** in the upper right corner of the dialog window.



For opening and closing the Results window, see *page 29*.

4.1.2 Terms


Control window	The main window 743 Rancimat Control is called the control window. It contains all the functions for monitoring and controlling the Rancimats connected to the PC.
Method	A method comprises all parameters for carrying out and evaluating a determination.
Determination	Determination refers to the automatic determination of the induction time and/or stability time for a sample. In order to carry out a determination, a method suitable for the samples must be selected.
Results	The results of a determination are automatically saved in the database Repos.mrd and can be viewed in the Results window .
Reevaluation	Reevaluation refers to the subsequent revision of a determination, in particular the manual specification of the induction time using tangents.
Recalculation	The recalculation can be used to subsequently recalculate results, formulas and standards.
Extrapolation	Extrapolation can be used to convert the results measured at various temperatures to a required target temperature. In addition, the factor for converting the induction time to the standard time can be determined.

4.1.3 Control window

The dialog window **743 Rancimat Control** serves for controlling the devices, managing methods, displaying the live curves and accessing various program functions. The dialog window opens automatically when the program is started.

Structure

The elements of the Control window are the **menu bar**, the **toolbar**, the **control panel** and the **status bar**.

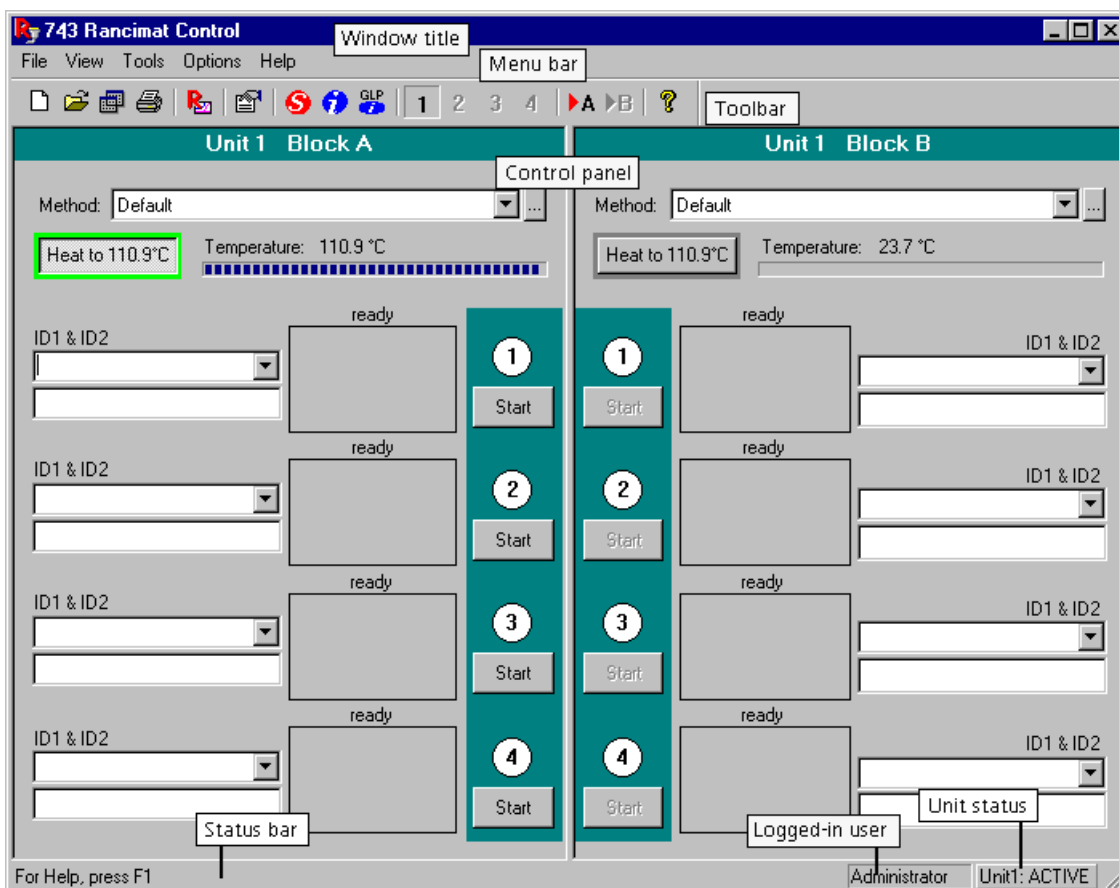

An image of the Rancimat is shown in the Control panel, which can be used for starting, displaying and stopping determinations.

The following information is shown in the status bar:

- a short description of the menu item highlighted in the menu bar
- the registered user
- the instrument status

Menus

The Control window contains the following main menus:














- | | |
|--------------|--|
| File | Create new methods, open existing methods, manage methods, open Results window, print, new login, close program. |
| View | Activate/Deactivate toolbar and status bar, display instrument information, change live parameters, display status overview, display event logging, select instrument. |
| Tools | Manage cell constants, perform GLP tests, set timer, set gas flow control, start all channels, determine Delta T, record temperature, perform service diagnosis. |



Options Carry out general settings, set instrument configuration, manage access rights.

Help Call up program-specific Online help.

Symbols

 New method	Create a new method (<i>see chapter 4.5.1, page 56</i>).
 Open method	Open an existing method (<i>see chapter 4.5.1, page 56</i>).
 Method Manager	Open, rename and delete methods (<i>see chapter 4.5.1, page 56</i>).
 Print	Print results (<i>see chapter 4.7.6, page 129</i>).
 Results	Open Results window (<i>see "Opening and closing the Results window", page 29</i>).
 Live parameters	Display live parameters which can be changed for a current determination (<i>see chapter 4.6.6, page 85</i>).
 Status overview	Display status overview for the instruments connected (<i>see chapter 4.3.2, page 45</i>).
 Instrument information	Instrument information (<i>see chapter 4.3.1, page 43</i>).
 GLP status	Display GLP status (<i>see chapter 4.8.3, page 145</i>).
 Instrument 1...4	Select instrument 1...4.
 Start all channels Block A	Start all channels of Block A (<i>see chapter 4.6.4, page 84</i>).
 Start all channels Block B	Start all channels of Block B (<i>see chapter 4.6.4, page 84</i>).
 Help topics	Call up the Online help.


4.1.4 Results window

The dialog window **743 Rancimat Results** serves for displaying, outputting and recalculating results of the determinations recorded with the 743 Rancimat. The determination data is saved in database files ***.mrd** and can be displayed in this dialog window in the form of overview tables and curves. The Results window can also run if the Control window is closed.

Opening and closing the Results window

Proceed as follows to open and close the Results window:

1 Open Results window

- In the dialog window **743 Rancimat Control**, click on the menu item **File ► Results...** or the symbol .


When opening the Results window, the database **Repos.mrd** is automatically loaded, in which all recorded determinations are saved by default.

2 Close Results window

- In the dialog window **743 Rancimat Results**, click on the menu item **File ► Back** or the symbol .

Structure

The elements of the Results window are the **menu bar**, the **toolbar**, the **subwindows** (determination overview, live, single and multiple graphs) and the **status bar**.

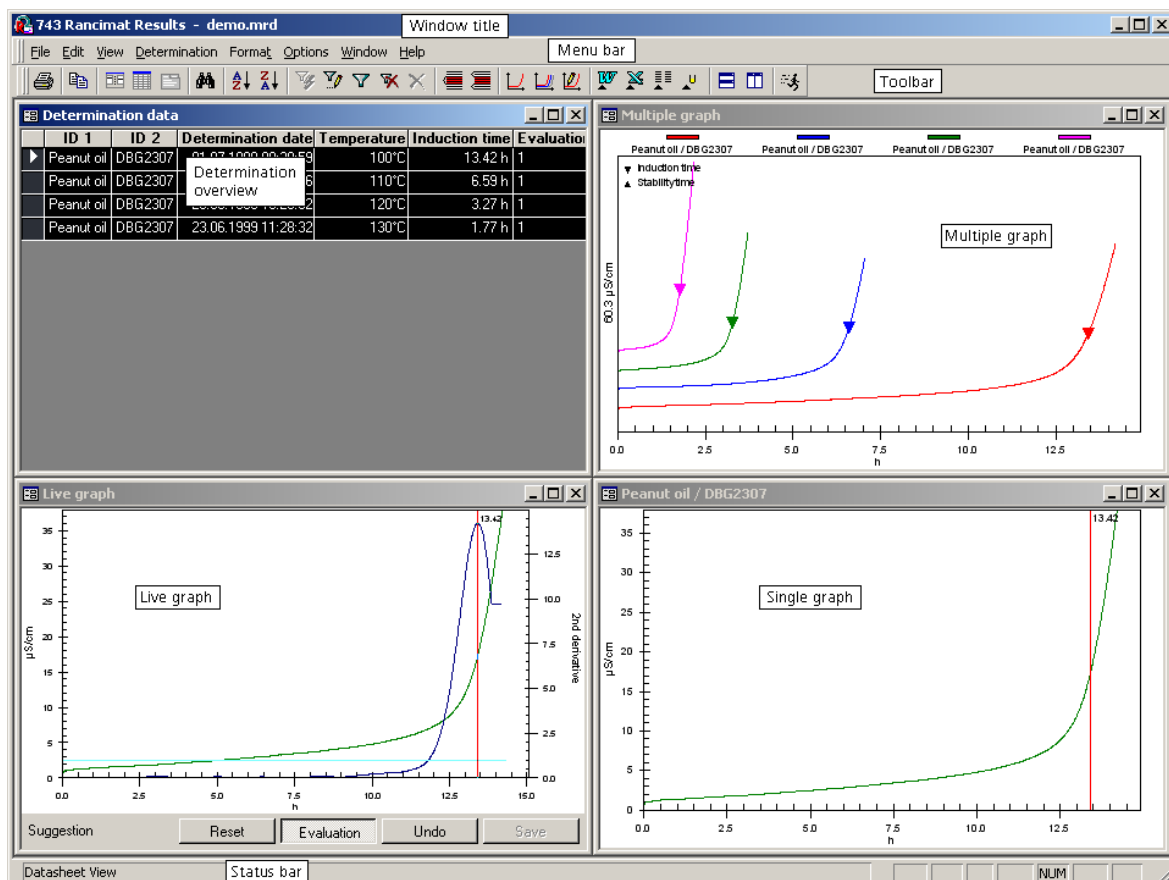



In the Results window subwindows with a determination overview, single, multiple or live graphs can be opened.










Menus

















The Results window contains the following main menus:

File	Open database, print, close dialog window.
Edit	Copy, select, delete content of the filter.
View	View selection: determination overview, determination and method data, GLP.
Determination	Search, sort, filter, display graphs, perform extrapolation, perform recalculation, export determinations, delete determinations.
Format	Format determination overview.
Options	Carry out general program settings.
Window	Arrange subwindows.
Help	Display program-specific Online help.

Symbols

The toolbar of the Results window contains the following symbols:

 Print	Print results, curves and overview lists (<i>see chapter 4.7.6, page 129</i>).
 Copy	Copy data to clipboard.
 Select fields for determination overview	Format determination overview (<i>see chapter 4.7.1, page 88</i>).
 Display determination overview	Display determination overview (<i>see chapter 4.7.1, page 88</i>).
 Display all methods and determination data	Display all methods and determination data of the selected determination (<i>see chapter 4.7.2, page 104</i>).
 Search	Search in the database (<i>see chapter 4.7.1, page 88</i>).
 Ascending	Sort column in ascending order (<i>see chapter 4.7.1, page 88</i>).
 Descending	Sort column in descending order (<i>see chapter 4.7.1, page 88</i>).
 Selection-based filter	Filter by selection (<i>see chapter 4.7.1, page 88</i>).

 Special filter	Define filter (see chapter 4.7.1, page 88).
 Apply filter	Apply filter (see chapter 4.7.1, page 88).
 Remove filter	Remove filter (see chapter 4.7.1, page 88).
 Delete filter	Delete content of the filter (see chapter 4.7.1, page 88).
 Filter selection	Only display selected determinations (see chapter 4.7.1, page 88).
 Selection not in filter	Hide selected determinations (see chapter 4.7.1, page 88).
 Single graph	Display single graph (see chapter 4.7.3, page 113).
 Multiple graph	Display multiple graph (see chapter 4.7.3, page 113).
 Live graph with reevaluation	Reevaluate live graph (see chapter 4.7.3, page 113).
 Export to Word	Export Determination overview to Word (see chapter 4.7.6, page 129).
 Export to Excel	Export Determination overview to Excel (see chapter 4.7.6, page 129).
 Export measured values	Export measured values to a TXT file (see chapter 4.7.6, page 129).
 Export determination and method data	Export determination and method data to a TXT file (see chapter 4.7.6, page 129).
 Tile vertically	Arrange subwindows on top of each other (see chapter 4.7.8, page 142).
 Tile horizontally	Arrange subwindows beside each other (see chapter 4.7.8, page 142).
 Return to main program	Close Results window and return to main program.

4.1.5 File types

The following file types are generated by the program 743 Rancimat:

***.mrd**

Database file

This file contains the measured data and results of the determinations. The file **repos.mrd** is automatically saved in the directory **Database**. When exporting databases, the memory location can be freely selected.

***.mel****Event file**

This file contains a protocol of all events which have occurred with the connected Rancimat. The file ***.mel** is automatically saved in the **Log** directory.

.txt*Text file**

Measured values, determination and method data as well as the data of the temperature log can be saved in ASCII format as a **TXT file**. The memory location can be freely selected, except for the temperature log. This file is saved in the **Log** directory.

4.1.6 Context-sensitive menus

Many menu functions of the Program window can also be selected by clicking with the right mouse button on the required dialog window or element. The menu options opened depend on the active dialog window or element selected.

4.1.7 Mouse functions

The standard functions for program control such as selecting menu items and fields can be executed using the mouse.

It also serves for magnifying a curve sector (Zooming).

Zooming

Proceed as follows:


1 Drag zoom square

- Place the cursor on the upper left corner of the sector to be magnified.
- Keeping the left mouse button pressed down, pull the cursor to the lower right corner of the sector.

The cursor assumes the form of a magnifying glass.

2 Release mouse button

- Release the mouse button in order to magnify the selected area to the full size of the window.

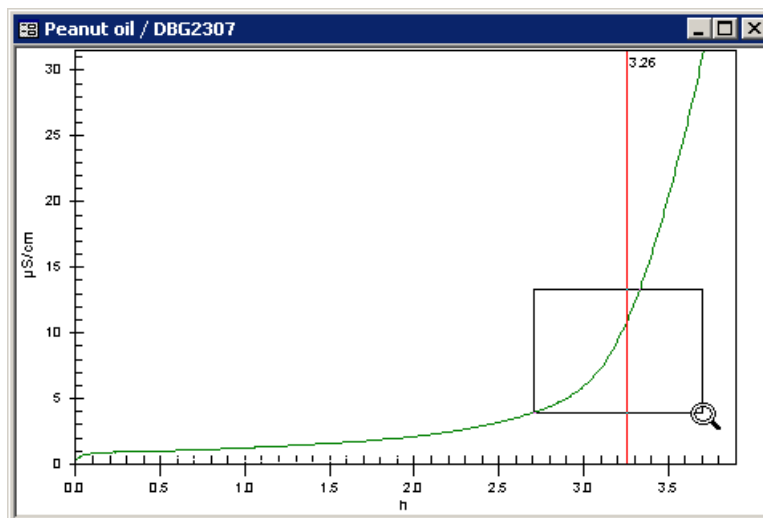

3 Switch zoom off again

- Right click in the graphs window.
The context-sensitive menu for graphs appears.
- Click on the menu item **Zoom Off**.

4.1.8 Help

You can call up help for the current topic anywhere with the symbol , the menu item **Help ► Help topics** or the key **[F1]**.

Green text	can be clicked on. This takes you to another help topic.
Violet text	marks menu items, parameters or buttons in the program.
Blue text	marks titles and important information.

- If a softswitch is used, activate the option **Softswitch in use** and select the serial interface of the softswitch to which the instrument is connected under **Softswitch port**.
- Confirm the entry with **[OK]**.

3 Restart program

- Close the program with the menu item **File ▶ Exit**.
- In the Windows Start menu under **Programs ▶ Metrohm ▶ Rancimat**, click on the menu item **Rancimat**.
- Enter the Administrator password and confirm with **[OK]**.


The program is opened. The message **Instr.#: Ready** now appears in the status bar for all connected instruments.

4.2.2 Managing access rights

The **743 Rancimat** program offers extensive password protection, allowing each menu item to be provided with individual access rights.

The dialog **Users and groups manager**, used to manage the access rights, is only accessible to the Administrator. The Administrator himself is not listed as a user, but has all access rights.

First of all, the access rights are given to different **Groups**. Then, individual **Users** can be assigned to a specific group.

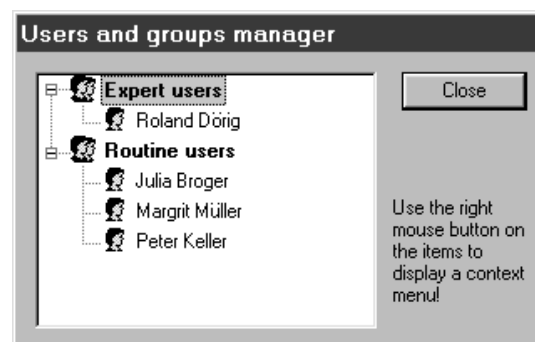

NOTICE

User lists are best created and passwords are best entered immediately after the first program start.

The setup for the users and their access rights is carried out in the following order:

1. Add a new group
2. Adjust rights for this group
3. Create users in this group



After having entered the access rights, the Login window for selecting the user and entering the password appears each time the program is started. All methods, determinations and reports are marked with the user name. It is possible to change the user at any time with the menu item **File ▶ New login...**

Adding a new group

In order to add a new group, proceed as follows:

1 Open Users and groups manager

- In the **Control window**, click on the menu item **Options ▶ User permissions...**

2 Create new group

- Right click on an existing group to select the menu item **Add group...**
- Under **Enter new group name** enter the name for the group and confirm with **[OK]**.

Adjusting access rights for the group

Proceed as follows to set the access rights:


1 Open Users and groups manager

- In the **Control window**, click on the menu item **Options ▶ User permissions...**

2 Open Properties dialog

- Right click on the relevant group whose access rights are to be adjusted to select the menu item **Properties...**

The following dialog window appears:

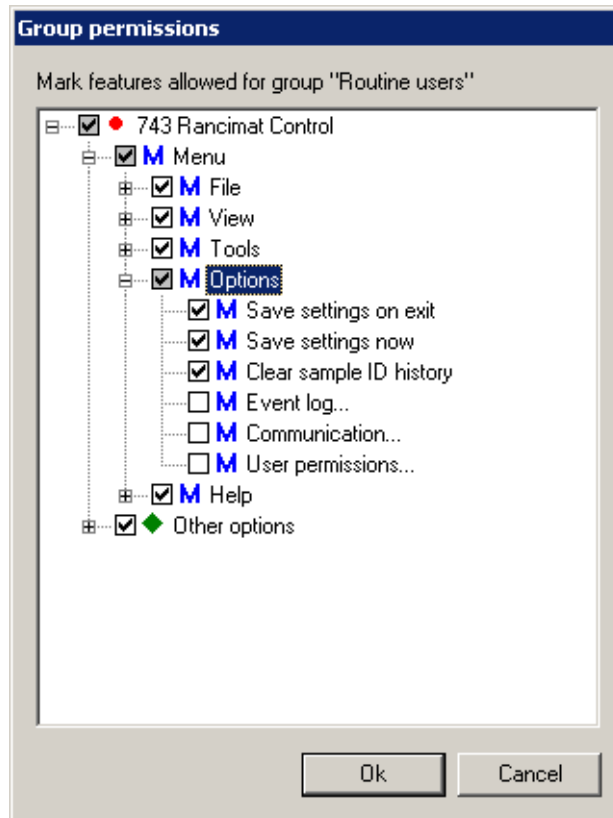

3 Activate/Deactivate the rights

- Click on the symbol to open the menu tree for the access rights..
- Activate or deactivate the required options by clicking on the symbol .
- Confirm the changes with **[OK]**.

Adding a new user

Proceed as follows to add a new user:

1 Open Users and groups manager

- In the **Control window**, click on the menu item **Options ► User permissions...**

2 Create new user

- Right click on an existing group to select the menu item **Add user...**
- Under **Enter new user name** enter the name for the user and confirm with **[OK]**.



Deleting a user

Proceed as follows to delete an existing user:

1 Open Users and groups manager

- In the **Control window**, click on the menu item **Options ▶ User permissions....**

2 Delete user

- Right click on the user to be deleted to activate the menu item **Delete user**.
- Confirm the message **Do you really want to delete user "user name"?** with **[Yes]**.

Deleting a group

Proceed as follows to delete an existing group:

1 Open Users and groups manager

- In the **Control window**, click on the menu item **Options ▶ User permissions....**

2 Delete group

- Right click on the group to be deleted in order to select the menu item **Delete group**.
- Confirm the message **Do you really want to delete group "group name"?** with **[Yes]**.

4.2.3 Timer

The function **Timer** can be used to start the two heating blocks A and B, independently of one another, automatically and at a time specified by you. The Rancimat has to be switched on and the software must be running.

Two different examples will explain how to program the timer.


Starting heating block A once automatically

Proceed as follows to automatically start the heating of block A at a specific time:

1 Open dialog window

- In the **Control window**, click on the menu item **Tools ▶ Timer function....**

The following dialog window appears:

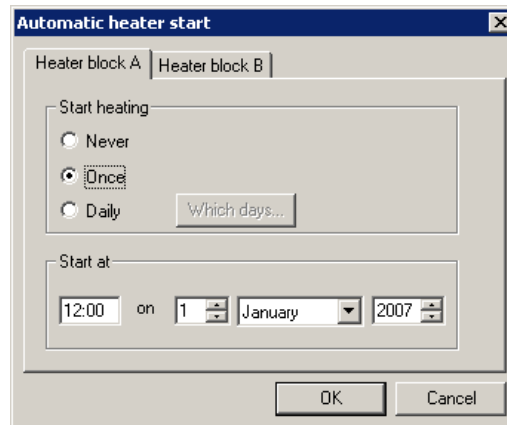

2 Set automatic start time

- Under **Start heating** select the option **Once**.
- Under **Start at...** enter the required time and date.
- Confirm the entries with **[OK]**.


Starting heating block B daily automatically at the same time

Proceed as follows to automatically start the heating of block B on a specific day of the week, at a specific time:

1 Open dialog window

- In the **Control window**, click on the menu item **Tools ▶ Timer function....**


The following dialog window appears:

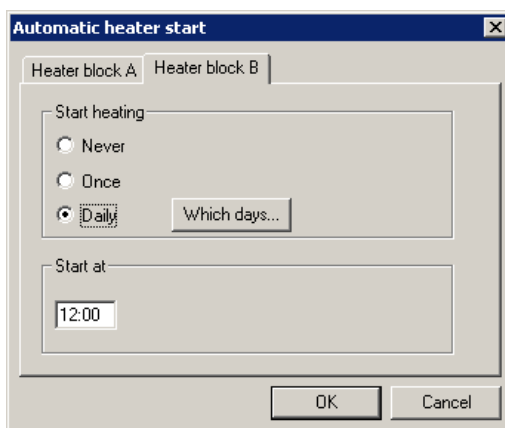

2 Set automatic start time

- Under **Start heating** select the option **Daily**.
- Click on the button **[Which days...]**.

The following dialog window appears:

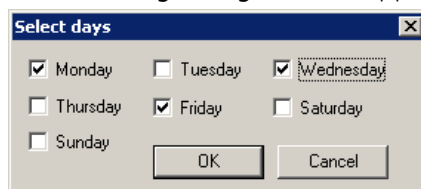

- Select the required day(s) and confirm with **[OK]**.
- Under **Start at...** enter the required time and confirm with **[OK]**.

4.2.4 Gas flow control

The gas flow produced by the **internal pump** through the reaction vessels to the measuring vessels can be switched on and off manually and displayed in a separate window.

Switching the gas flow on and off

Proceed as follows:

1 Switch on

- Click on the menu item **Tools ▶ Gas flow control ▶ Gas flow on**.

2 Switch off

- Click on the menu item **Tools ▶ Gas flow control ▶ Gas flow off**.


Displaying the gas flow

Proceed as follows:

1 Open dialog window

- Click on the menu item **Tools ▶ Gas flow control ▶ Display gas flow...**

The following dialog window appears:

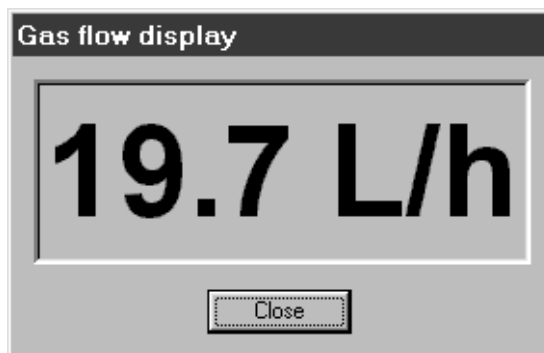

NOTICE

This option is only available if no determination is running.

4.2.5 Recording the temperature

The temperature can be recorded at any time for each individual heating block.

The program writes the recorded measured values into a text file containing the following values:

t(s)	Time in seconds.
Block [°C]	Temperature measured in the heating block.
Ext. Sensor [°C]	Temperature measured with the external temperature sensor.

The text file is saved under the name **U#X-YYMMDD-hhmmss.txt** in the folder **Log**, # denoting the instrument number (1...4), X denoting the block (A or B) and YYMMDD-hhmmss denoting the date and time when the data logging started.



Switching the temperature log on and off

Proceed as follows:

1 Switch on the recording for block A or B

- Click on the menu item **Tools ▶ Temp. logging ▶ Block A on.**

or

- Click on the menu item **Tools ▶ Temp. logging ▶ Block B on.**

2 Switch off the recording for block A or B

- Click on the menu item **Tools ▶ Temp. logging ▶ Block A off.**

or

- Click on the menu item **Tools ▶ Temp. logging ▶ Block B off.**

4.2.6 Optimizing program and database

The data which the program **Rancimat** requires for displaying the Results window is saved in the file **Nachaus.prg**. With the standard installation, this file is located at C:\Program Files\Metrohm\Rancimat\Template. As soon as the file is **greater than 10 MB**, you should optimize and compress the program, so that this file no longer has any superfluous data and the program runs faster again.

The **file size of the database Repos.mrd** can make access to existing determinations considerably slower. If you regularly work with the program and carry out a large amount of determinations, you should optimize the standard database **Repos.mrd** once a month.

Optimizing the program

Proceed as follows to optimize the program:

1 Quit program

- Close the program **Rancimat** (*see chapter 4.1.1, page 25*).

2 Optimize program

- In the windows Start menu, click on the menu item **Programs ▶ Metrohm ▶ Rancimat ▶ Optimize ▶ Program.**

Optimizing the database

Proceed as follows to optimize the standard database:

1 Export database

- Export determinations not currently required from the database **Repos.mrd** into a newly created database (see "Exporting determinations to another database", page 134).
- Close the Results window and the program **Rancimat** (see chapter 4.1.1, page 25).

2 Optimize database

- In the Windows Start menu, click on the menu item **Programs ▶ Metrohm ▶ Rancimat ▶ Optimize ▶ Database**.

4.3 Program information

4.3.1 Instrument information

Displaying and printing the instrument information

Proceed as follows to display and print the instrument information of the currently selected Rancimat:

1 Open dialog window

- In the **Control window**, click on the menu item **View ▶ Unit information....**

The following dialog window appears:



2 Print instrument information

- Click on the button **[Print report...]**.

The status report is printed on the printer which is defined on your PC as the default printer.

Meaning of the individual parameters

Serial number

Serial number of the selected instrument.

Program number

Number of the EEPROM program of the selected instrument.

Last maintenance

Date of the last maintenance with signature of the service technician who has carried out the service work.

Last calibration

Date of the last instrument adjustment with signature and code of the responsible body.

Unit operating hours

Number of hours during which the instrument was switched on.

Pump operating hours

Number of hours during which the internal pump was in operation.

**NOTICE**

The block **Service diagnosis** is password-protected and only accessible for trained service personnel.

4.3.2 Status overview

Displaying the status overview

Proceed as follows to display and adjust the status overview:

1 Open dialog window

- In the **Control window**, click on the menu item **View ▶ Status overview**.

The following dialog window appears:

Unit	Block	Channel	Method	Sample ID1	Status	Stab. time	Induc. time	Set temp.	Current temp.
1	A	1	Default		ready			121.60°C	23.29°C
1	A	2	Default		ready			121.60°C	23.29°C
1	A	3	Default		ready			121.60°C	23.29°C
1	A	4	Default		ready			121.60°C	23.29°C
1	B	1	Default		ready			121.60°C	22.88°C
1	B	2	Default		ready			121.60°C	22.88°C
1	B	3	Default		ready			121.60°C	22.88°C
1	B	4	Default		ready			121.60°C	22.88°C

2 Adjust and save column width

- You can adjust the column width to the required size by dragging the right field border with the mouse.
- In the **Control window**, click on the menu item **Options ▶ Save settings now**.

Meaning of the columns in the status overview

Unit

Instrument number (1...4).

Block

Instrument block (A or B).

Channel

Channel (1...4).

Method

Name of the method loaded.

**Sample ID1**

Sample identification 1.

Status

Status of the channel.

ready: No active measurement. The channel is ready for starting a determination.

running: Instrument is measuring.

finished: Determination finished. The channel is ready for starting a new determination.

error: Communication error between instrument and PC.

Stab. time

Stability time determined.

Induc. time

Induction time determined.

Set temp.

Setpoint temperature (defined in the method).

Current temp.

Current block temperature.

4.3.3 Displaying, filtering and deleting event overview**Opening and saving the event log file**

Proceed as follows to display and save all events of the Rancimat connected to the PC:

1 Open current log file

- In the **Control window**, click on the menu item **View ► Event log overview**.

The following dialog window appears:

The screenshot shows the MLogView application window with a menu bar (File, View, Filter, Help) and a toolbar. The main area contains a table of log entries with the following columns: T., Date, Time, User, Unit, and Event. The entries are as follows:


T.	Date	Time	User	Unit	Event
i	04.01.2007	11:25:55	Administrator	1	Method "Default" selected for Block A
!	04.01.2007	11:25:55	Administrator	1	Different gas flow setting for block A and B (A r
i	04.01.2007	11:25:49	Administrator	1	Method "Default" saved
i	04.01.2007	11:23:46	Administrator	1	Connection established (serial no. 1122)
i	04.01.2007	11:23:44	Administrator	n.a.	User "Administrator" logged in
i	04.01.2007	11:23:43	n.a.	n.a.	Program start
i	04.01.2007	11:23:42	Administrator	n.a.	Program closed
i	04.01.2007	11:23:39	Administrator	n.a.	Unit configuration changed
i	04.01.2007	11:23:32	Administrator	n.a.	User "Administrator" logged in
i	04.01.2007	11:23:32	n.a.	n.a.	Program start
i	04.01.2007	11:23:11	Administrator	n.a.	Program closed
!	04.01.2007	11:22:48	Administrator	1	Wrong unit type connected
i	04.01.2007	11:22:36	Administrator	n.a.	User "Administrator" logged in




NOTICE

You can find the meaning of the symbols and columns in the event overview at "*Meaning of the symbols and columns in the event overview*", page 48.


2 Update view

- Click on the symbol  or the menu item **View ► Refresh** to view the current status of the log file.

3 Save log file

- Click on the symbol  or the menu item **File ► Save as....**
- In the dialog window **Save file as** enter a **file name** and confirm with **[OK]**.

4 Open saved log file

- Click on the symbol  or the menu item **File ► Open....**
- In the dialog window **Open**, select the required file and confirm with **[OK]**.

Filtering entries in the event overview

Proceed as follows to filter the entries in the event file:

1 Filter the entries

- Click on the required filter criterion (e.g.: date = "30.08.2006").

Time

Time of the event. The format depends on the settings defined in Windows in **Control Panel ▶ Country settings ▶ Time**.

User

Name of the user logged in at the time of the event.

Unit

Instrument number (1...4).

Event

Description of the event.

4.4 Calibration functions

4.4.1 Determining cell constants

Only the **change in conductivity** is measured and evaluated during the Rancimat measurement. As a result, the cell constants of the conductivity measuring cells used in the Rancimat, which are normally in the range from 1.00...1.20, only have to be entered exactly if the **absolute conductivity measured value** is to be displayed correctly.

The value also has to be entered before carrying out the **GLP test "Conductivity"**. The cell constants can thereby be entered manually or determined automatically using a defined standard solution.


Entering cell constants manually

Proceed as follows if you wish to enter the cell constants manually:

1 Open dialog window

- Click on the menu item **Tools ▶ Cell constants ▶ Manual...**

The following dialog window appears:

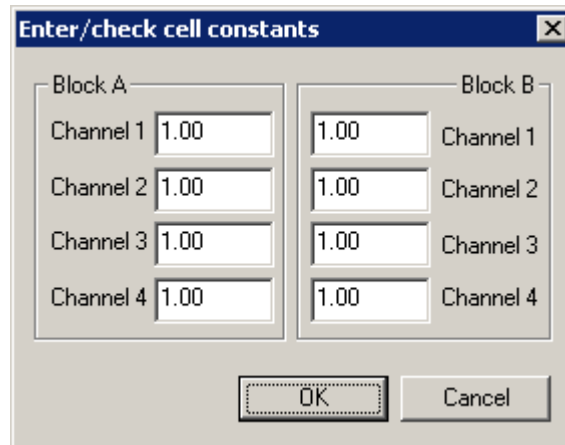

2 Enter cell constants

- Enter the cell constants of the conductivity measuring cells for the required channels and confirm with **[OK]**.


Determining cell constants automatically

Proceed as follows if you wish to enter the cell constants automatically:

1 Open dialog window

- Click on the menu item **Tools ▶ Cell constants ▶ Automatic....**

The following dialog window appears:

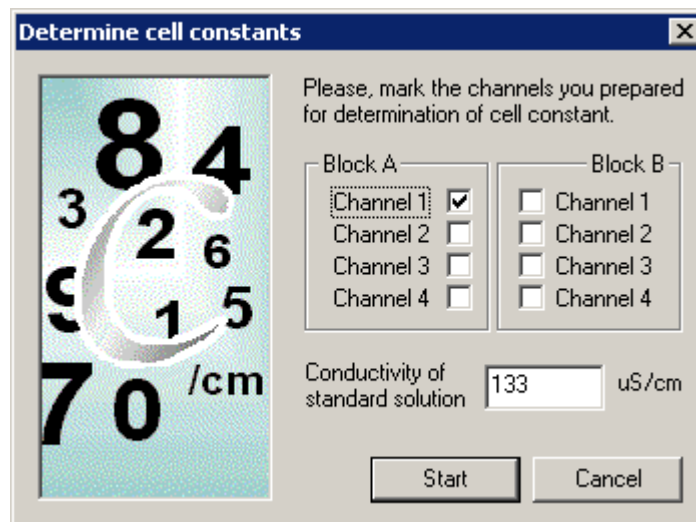

2 Select channels and define conductivity

- Activate the check boxes of those channels, for which the cell constant is to be determined.

- Enter the conductivity of the standard used.

c(KCl) = 1 mmol/L can be used as a standard solution. This is derived from the optionally available conductivity standard 6.2301.060 (KCl 0.1 mol/L) through dilution with distilled water. The conductivity of this diluted solution is:

Temperature	Conductivity
18 °C	127 µS/cm
19 °C	130 µS/cm
20 °C	133 µS/cm
21 °C	136 µS/cm
22 °C	138 µS/cm
23 °C	141 µS/cm
24 °C	144 µS/cm
25 °C	147 µS/cm

Alternatively, the conductivity standard 6.2324.000 (undiluted) can be used.

3 Start determination and check the values

- Click on **[Start]** to start the determination of the cell constant.

After the determination is finished, the dialog window **Enter/Check cell constants** appears again.

If you wish to accept the displayed values, click **[OK]**.

If you wish to maintain the old values, click **[Cancel]**.

4.4.2 Determining Delta T

The **temperature correction Delta T** indicates the deviation of the current temperature of the sample from the temperature in the heating block and belongs to the method as a parameter (*see chapter 4.5.2, page 61*). It can automatically be determined with the calibrated, external temperature sensor (part of the optionally available GLP test set,).

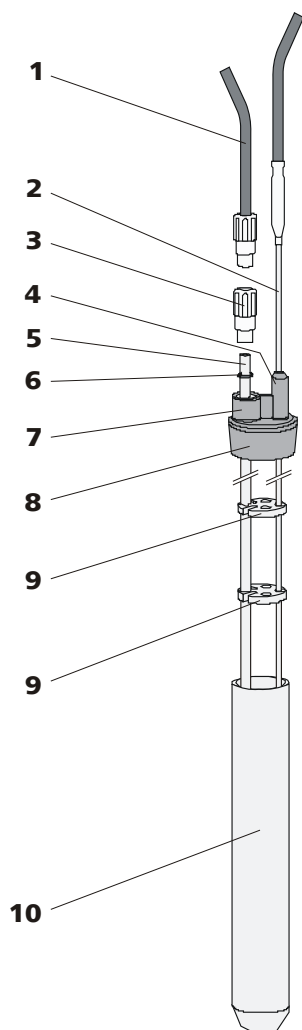


Figure 6 Equipping the reaction vessel for determining Delta T

1	FEP tubing 250 mm (6.1805.080) For supplying air into the reaction vessel.	2	Pt100 temperature sensor
3	Thread adapter M8 / M6 (6.1808.090)	4	Opening for temperature sensor For inserting the temperature sensor.
5	Air tube	6	O-ring (6.1454.040)
7	Connector For connecting the thread adapter M8 / M6.	8	Reaction vessel cover (6.2753.107)
9	Spacer (6.2042.040)	10	Reaction vessel (6.1429.040)

Preparing Delta T determination

Figure 6 shows in detail how the accessories for determining Delta T are mounted. Proceed as follows:

1 Prepare reaction vessel cover

- Mount the air tube on the reaction vessel cover (see "Mount the reaction vessel cover", page 15).
- Clamp the first spacer at a distance of approx. 12 cm from the lower end onto the air tube.
- Clamp the second spacer at a distance of approx. 5 cm from the lower end onto the air tube.
- Insert the temperature sensor from above into the temperature sensor opening of the reaction vessel cover and fasten it in the corresponding openings of the spacers.

2 Prepare reaction vessel

- Fill the reaction vessel with 5 g silicone oil (e.g. FLUKA 85409).
- Place the reaction vessel cover with the temperature sensor on the reaction vessel.
- Push the temperature sensor fully downwards (the sensor must be on the vessel base).

3 Insert and connect reaction vessel

- Insert the reaction vessel with the mounted reaction vessel cover in channel 2 or 3 of the required heating block.
- Screw the one end of the FEP tubing 250 mm onto the thread adapter M8 / M6 of the reaction vessel cover.
- Screw the other end of the FEP tubing onto the corresponding connector (3-3) of the Rancimat.

4 Set method parameters




NOTICE

Create a unique method for both blocks, so that you can separately enter the temperature correction for both blocks.

- In the **Control window**, select the required **method** for the heating block for which the temperature correction Delta T is to be determined (see "Select method", page 82).



- Click on the symbol . The dialog window with the method parameters is opened.
- Under **Temperature** enter the required setpoint temperature for the sample and set **Delta T** to 0 °C.
- Set the **gas flow** to the required value and finalize with **[Save]**.

5 Start gas flow and heating

- Click on the menu item **Tools ▶ Gas flow control ▶ Gas flow on**.
- Click on the button **[Heat to xx °C]**.


Executing a Delta T determination

After you have prepared everything for determining Delta T (see "Preparing Delta T determination", page 53), you can now execute the determination of Delta T as follows:

1 Enter sensor calibration data

- Click on the menu item **Tools ▶ Determine Delta T ▶ Block A** or **Block B**.

The following dialog window appears:

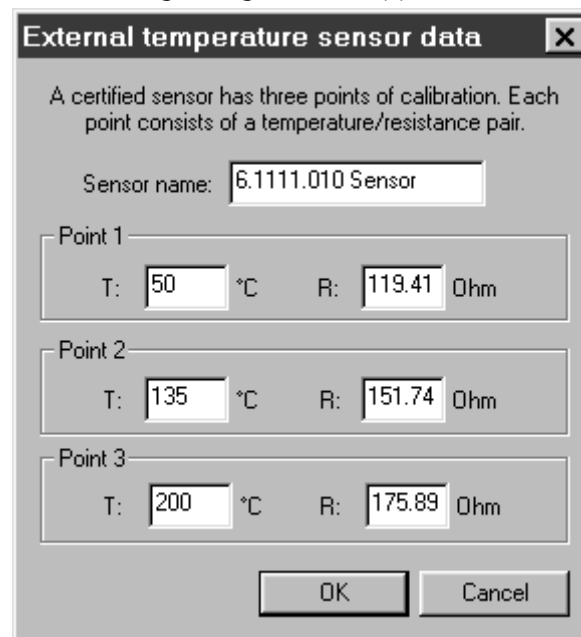

External temperature sensor data [X]

A certified sensor has three points of calibration. Each point consists of a temperature/resistance pair.

Sensor name: 6.1111.010 Sensor

Point 1
T: 50 °C R: 119.41 Ohm

Point 2
T: 135 °C R: 151.74 Ohm

Point 3
T: 200 °C R: 175.89 Ohm

OK Cancel


- Enter a **Sensor name**.
- Enter the calibration data (temperature and resistance) for **Points 1 to 3** and confirm with **[OK]**.



NOTICE

You can find the calibration data (T1 to T3) for Metrohm sensors on the certificate enclosed with the sensor or on the label fastened on the sensor cable.

The following dialog window appears:

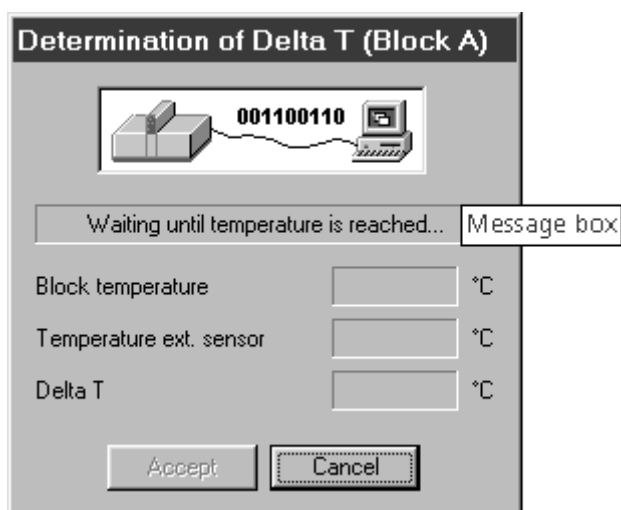

2 Wait for measurement

- Wait until the message **Measured temperature is now stable!** appears in the message box.

The following three values are displayed below the message box:

Block temperature	Temperature which has been measured in the heating block with the internal temperature sensor.
Temperature of ext. sensor	Temperature which has been measured in the reaction vessel with the external temperature sensor.
Delta T	Temperature correction which is determined from the difference between the block temperature and the temperature of the ext. sensor.

New method

Standards | Documentation | Description

Parameters | Evaluation | Curves | Formulas

Temperature: 120 °C Delta T: 1.6 °C

Gas flow: 20 L/h Use internal pump

Start options

Start delay: 0 min

Start mode: per channel per 2 channels per block

Stop criteria

Time 0 h Endpoint(s)

Conductivity >= 0 uS/cm

Shut off at end of determinations

Heater Gas flow

Save Save as... Print... Cancel

2 Adjust parameters

- Adjust the required parameters.
- Click on the tab **Evaluation** and also adjust the parameters.
- Repeat for all remaining tabs.



NOTICE

You can find a detailed description of all tabs and their parameters at *4.5.2 Parameter description*.

3 Save method


- Click on the **[Save as...]** button.
The dialog window **Save method as...** opens.
- Enter the method name and confirm with **[Save]**.



Opening a selected method and adjusting parameters

Proceed as follows to open the method which is selected in the **Control window** and adjust its parameters:

1 Open method

- In the **Control window**, click on the symbol  in the required **Block A** or **B**.
The dialog window "**Method name**" appears.


2 Adjust parameters and save changes

- Adjust the parameters (*see chapter 4.5.2, page 61*).
- Confirm the changes with **[Save]**.

Opening an existing method and adjusting parameters

Proceed as follows to open an existing method and adjust its parameters:

1 Open existing method

- In the **Control window**, click on the symbol  or the menu item **File ▶ Open method...**.
The dialog window **Open method** appears.
- Click on the required method and confirm the selection with **[Open]**.

The dialog window "**Method name**" appears.

2 Adjust parameters and save changes

- Adjust the parameters (*see chapter 4.5.2, page 61*).
- Confirm the changes with **[Save]**.

Renaming an existing method


Proceed as follows to rename an existing method:




NOTICE

A method which is still selected in one of the blocks A or B, cannot be renamed. Select another method first in order to rename the required method.

1 Open Method manager

- In the **Control window**, click on the symbol  or the menu item **File ► Method manager...**

The following dialog window appears:

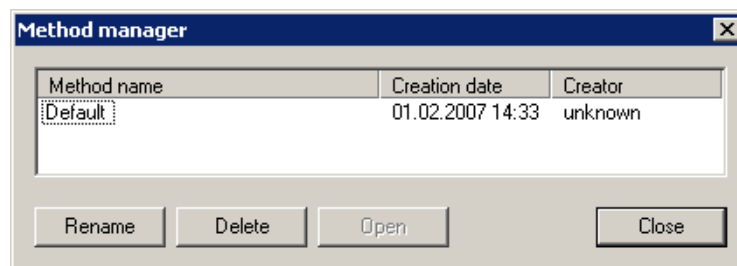


2 Select and rename method

- Click on the required method and then the button **[Rename]**. The method name is highlighted in blue.
- Enter the new method name and click with the mouse on the free white area below the method name in order to accept the change.
- Click on the **[Close]** button.

Saving a method under a new name

Proceed as follows to save an existing method under a new name:

1 Open method

- In the **Control window**, click on the symbol  or the menu item **File ► Open method...**. The dialog window **Open method** appears.
- Click on the required method and confirm the selection with **[Open]**.

The dialog window "**Method name**" appears.



2 Save it with a new name

- If necessary, adjust the parameters (*see chapter 4.5.2, page 61*).
- Click on the **[Save as...]** button.
The dialog window **Save method as...** appears.
- Enter the method name and confirm with **[Save]**.

Deleting an existing method


Proceed as follows to delete an existing method:




NOTICE

A method which is still selected in one of the blocks A or B, cannot be deleted. Select another method first in order to delete the required method.

1 Open Method manager

- In the **Control window**, click on the symbol  or the menu item **File ► Method manager...**

The following dialog window appears:

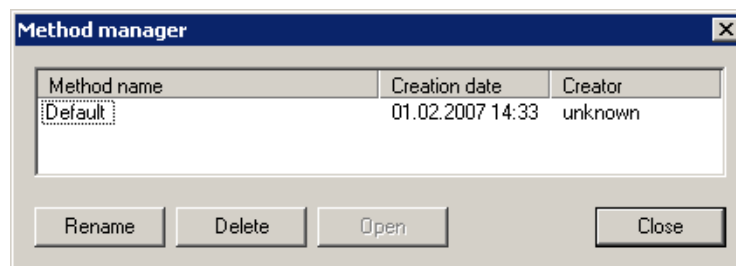


2 Select and delete method

- Click on the required method and then the button **[Delete]**.
The safety prompt "**Do you really want to delete method "method name"?**" appears.
- Confirm the safety prompt with **[Yes]**.

Printing parameters of a method

Proceed as follows to print the parameters of an existing method:

1 Open method

- In the **Control window**, click on the symbol  or the menu item **File ▶ Open method...**
The dialog window **Open method** appears.
- Click on the required method and confirm the selection with **[Open]**.

The dialog window "**Method name**" appears.

2 Print parameters

- Click on the **[Print...]** button.
The dialog window **Print Setup** opens. All the printers installed on your PC appear under **Name**.
- Select the required printer and confirm with **[OK]**.

4.5.2 Parameter description

A method contains several parameters which are distributed on various tabs. This section explains all the parameters, arranged according to tab.

4.5.2.1 "Parameters" tab

The most important parameters (temperature, gas flow, Delta T) for carrying out the measurement are set using this tab. The settings affect the progression of the measurement curve recorded.

Temperature

Setpoint temperature of the sample.

Input range **50 - 220 °C**

Delta T

Temperature correction: indication of how much the block temperature has to be increased so that the sample reaches the setpoint temperature. This value is determined through measurement of the deviation by the current temperature of the sample from the heating block temperature using a calibrated, external temperature sensor (*see chapter 4.4.2, page 51*).



NOTICE

If no temperature sensor is available for determining Delta T, you can enter the approximate values listed in the table below, which have been determined with 5 g silicone oil and a gas flow of 20 L/h (air).

Input range **-9.9 - 9.9 °C**

Table 1 Approximate values for determining Delta T

Setpoint temperature	Delta T
80 °C	+1.1 °C
90 °C	+1.3 °C
100 °C	+1.4 °C
110 °C	+1.5 °C
120 °C	+1.6 °C
130 °C	+1.7 °C
140 °C	+1.8 °C
150 °C	+1.9 °C
160 °C	+2.0 °C

Gas flow

Gas flow through the sample. The gas flow can only be set for both blocks jointly. The value of the method loaded for block A is always decisive.

Input range	7 - 25 L/h
-------------	-------------------

Use internal pump

on | off (Default value: **on**)

Switch on/off gas supply with internal pump. If the internal pump is switched off, an external gas supply must be connected to the **Air/N₂ in** connection (see chapter 3.2.2, page 13).

Start options

Start delay

Waiting time until starting the measurement.

Input range	0 - 1000 min
-------------	---------------------

Start mode

Mode for starting and stopping the channels.

Selection	per channel per 2 channels per block
-----------	---

per channel

All channels can be started and stopped individually.

per 2 channels

2 channels each can be started and stopped jointly. The **[Start]** button in the control window changes automatically for this.

**per block**

The 4 channels of a block can be started and stopped jointly.

Stop criteria**Time**

on | off (Default value: **off**)

Time until the automatic stop of the determination.

Input range **0.1 - 9999 h**

Conductivity

on | off (Default value: **off**)

Conductivity limit value. If this value is reached, the determination is ended automatically.

Input range **1 - 400 µS/cm**

Endpoint(s)

on | off (Default value: **off**)

Automatic stop of the determination, as soon as every active channel has reached all endpoints (induction time and stability time).

Table 2 Overview of stop criteria

Time	Conductivity	Endpoint(s)	Analysis stops...
			not automatically.
✓			after the time entered, independently of reaching the induction/stability time (endpoint).
	✓		after reaching the conductivity entered, independently of reaching the induction/stability time (endpoint).
		✓	after reaching the induction and stability time (endpoint) defined on the Evaluation tab. If the induction and stability time are evaluated, both endpoints have to be found.
✓	✓		after reaching the first criterion (time or conductivity), independently of reaching the induction/stability time (endpoint).
✓		✓	after reaching the first criterion (time or endpoint). If the time entered has been reached, there is no further measuring until the induction/stability time (endpoint) has been reached.

Time	Conductivity	Endpoint(s)	Analysis stops...
	✓	✓	after reaching the first criterion (conductivity or endpoint). If the conductivity entered has been reached, there is no further measuring until the induction/stability time (endpoint) has been reached.
✓	✓	✓	after reaching the first criterion. If the time or conductivity entered has been reached, there is no further measuring until the induction/stability time (endpoint) has been reached.

Actions at end of determinations...

Shut off heater

on | off (Default value: **off**)

Automatic deactivation of the heating at the end of the determination.

Shut off gas flow

on | off (Default value: **off**)

Automatic deactivation of the gas flow at the end of the determination.




CAUTION

If the gas flow is automatically switched off, the reaction vessels must be removed from the instrument within 30 to 60 min after the end of the determination. If the vessels are not removed, a vacuum could develop over the course of time, which would thus result in back suction of the measuring solution into the hot reaction vessel.

4.5.2.2 "Evaluation" tab

These settings serve for automatic evaluation of the curve. After finishing the measurement, curves can also be reevaluated in the database (see chapter 4.7.3, page 113).

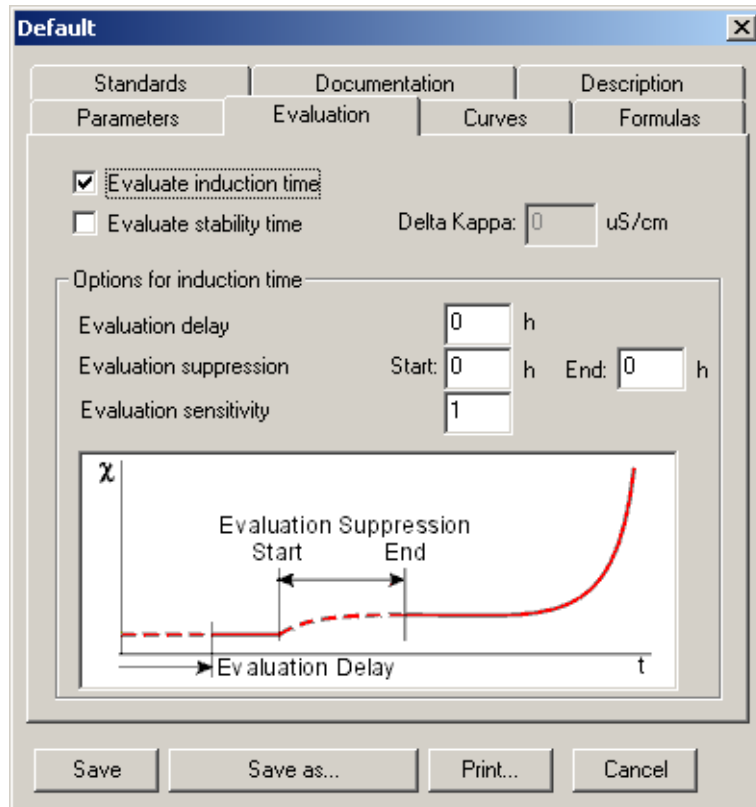

Evaluate induction time

on | off (Default value: **on**)

Determination of the **induction time** (see "Induction time", page 67).

Evaluate stability time

on | off (Default value: **off**)

Determination of the **stability time** (see "Stability time", page 68).



NOTICE

If you select this evaluation mode, you always need to calibrate the conductivity measuring cell beforehand.

Delta Kappa

Conductivity change for the determination of the stability time.

Input range	1 - 400 μS/cm
-------------	-------------------------------------

Options for induction time

Evaluation delay

Waiting time until starting the curve evaluation.

Input range	0 - 100 h
-------------	------------------

Evaluation suppression

Start

Time from the start of the determination to the start of the evaluation suppression.

Input range	0 - 100 h
-------------	------------------

End

Time from the start of the determination to the end of the evaluation suppression.

Input range	0 - 100 h
-------------	------------------

Evaluation sensitivity

This value defines the minimum value which the maximum of the curve of the second derivative has to reach in order to be accepted as a result. The result, i.e. the induction time, is the time until the first accepted maximum.


The default value "1" will lead to the correct result for most applications. Smaller values will cause the acceptance of smaller maximums of the second derivative. Higher values require a higher maximum.

Input range	0.1 - 9999
-------------	-------------------

Induction time

The induction time is the **time to the break point** of the curve *conductivity vs. time* recorded with the Rancimat. The induction time is a parameter for the oxidation stability of the sample examined and corresponds to a large extent to the results from the complex AOM method.


For automatic determination of the induction time, the second derivative of the measured curve is used, which exhibits a maximum at the break point and which can be displayed in the window **Live graph**. To enable detection of a break point, certain criteria must be fulfilled with regard to the height and width of the peak in the second derivative. The break point can also be determined manually as the intersection point of the two tangents at the extended straight branches of the curve (see "Setting tangents manually", page 117).

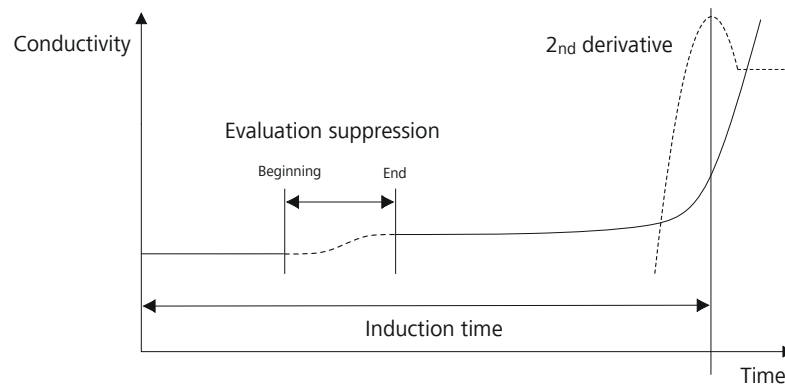

With certain samples, it may occur that the conductivity rises in steps, to a small degree, long before the actual induction time (e.g. through side reactions or with volatile compounds). To prevent this rise being evaluated as an endpoint, the user can delay the evaluation or suppress it for a certain range.

Stability time


The stability time is the time which is necessary in order to attain a specified **conductivity change Delta Kappa**.

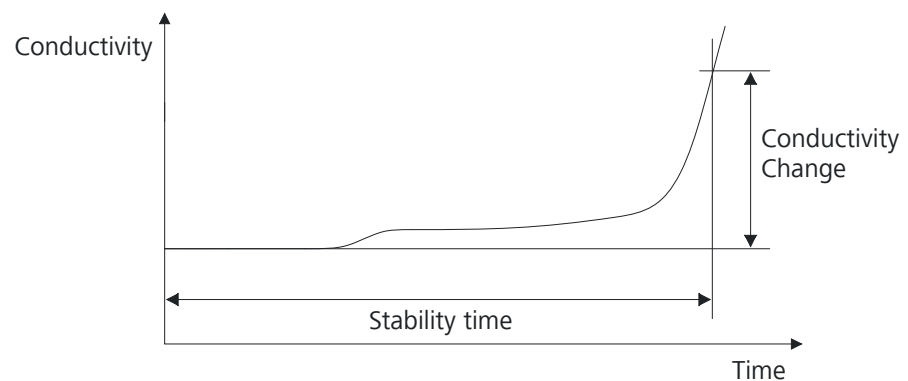

The entry of an evaluation delay or evaluation suppression does not have any effect on this evaluation mode. In all cases the time from the start point of the measurement is calculated.

4.5.2.3 "Curves" tab

The scaling of the x and y axis can be defined here. The settings have an effect on the expression of the curves, but not on the measurement and evaluation. After completing the determination, the scaling for single and live graphs can be changed again in the determination overview.

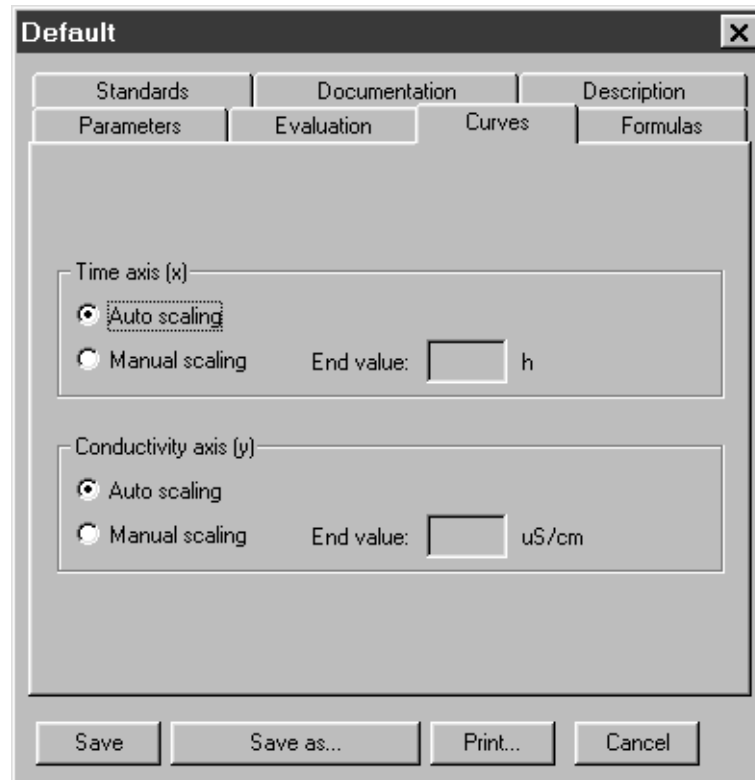**Time axis (x)**

Selection	Auto scaling Manual scaling
-----------	--------------------------------------

Auto scaling

Automatic definition of the start and end value of the time axis.

Manual scaling

Manual definition of the end value of the time axis.

End value

End value of the time axis with manual scaling.

Input range	0.5 - 100 h
-------------	--------------------

Conductivity axis (y)

Selection	Auto scaling Manual scaling
-----------	--------------------------------------

Auto scaling

Automatic definition of the start and end value of the conductivity axis.

Manual scaling

Manual definition of the end value of the conductivity axis.

End value

End value of the conductivity axis with manual scaling.


Input range	10 - 400 μS/cm
-------------	--------------------------------------

Formula 3 for stability time:**on | off** (Default value: **off**)

If this option is activated, the automatically determined stability time will be calculated with the entered values. The result will be saved under the name entered in the field "R3".

4.5.2.5 "Standards" tab

This function can be used to automatically calculate the induction time for a temperature deviating from the measuring temperature, the so-called standard time. The settings here do not have any effect on the measuring sequence or the evaluation. After finishing the measurement, a post-calculation or recalculation is possible at any time in the determination overview (see chapter 4.7.5, page 122).

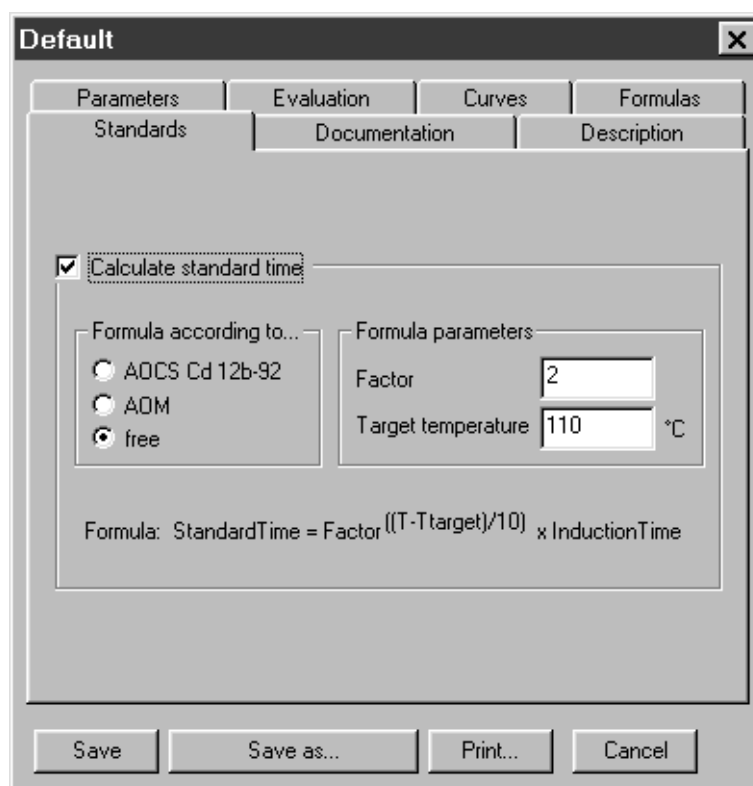**Calculate standard time****on | off** (Default value: **off**)

Activation/Deactivation of the calculation of the standard time according to the following formula:

$$\text{Standard time} = \text{Factor}^{(\text{Temperature} - \text{Target temperature})/10} \times \text{induction time}$$

Formula according to...

Selection	AOCS Cd12b-92 AOM free

Include in report...**Header****on | off** (Default value: **on**)

Output of the header with company settings (see *""Company settings" tab", page 138*), date of the printout, sample identifications, instrument information, determination date, user, cell constant and serial number.

Method parameters**on | off** (Default value: **on**)

Output of the method parameters.

Curve(s)**on | off** (Default value: **on**)

Output of the curves.

Method description**on | off** (Default value: **off**)

Output of the method description entered on the tab **Description**.

Results**on | off** (Default value: **on**)

Output of the selected results.

Selection	Induction time	Stability time	Standard time
	Formula 1	Formula 2	Formula 3

Automatic report output**Send to printer immediately****on | off** (Default value: **on**)

Automatic printout of the report defined under **Include in report...** after finishing the determination.

Send to file**on | off** (Default value: **off**)

Automatic output of determination and method data after finishing the determination as TXT file for further processing in other programs. The content of this report is independent of the report elements defined at **Include in report...**

Browse...

Selection of the directory for saving this file.



Example of an automatically printed report

Unit	1	Serial number	01109	Printing date	09.09.2006 09:34:03
Block	A	Cell constant	1	Determination date	23.06.2006 13:25:52
Channel	1	User	Administrator		

ID 1	ID 2
Peanut oil	DBG2307

Induction time	3.26 h
-----------------------	--------

Method name	Oil 120°C	Creation date	23.06.2006 08:27:20
Creator	Administrator		


Temperature	120 °C	Stop time	0.00 h
Delta T	1.60 °C	Stop at conductivity	0 µS/cm
Gas flow	20 L/h	Stop at endpoint	<input checked="" type="checkbox"/>
Start delay	0 min	Delta Kappa	0 µS/cm
Start mode	<input checked="" type="radio"/> per channel <input type="radio"/> per 2 channels <input type="radio"/> per block	Evaluation delay	0.00 h
		Evaluation delay start	0.00 h
		Evaluation delay end	0.00 h

Send to file

GLP test passed.


4.5.2.7 "Description" tab

You can enter a comment on the method in this tab.

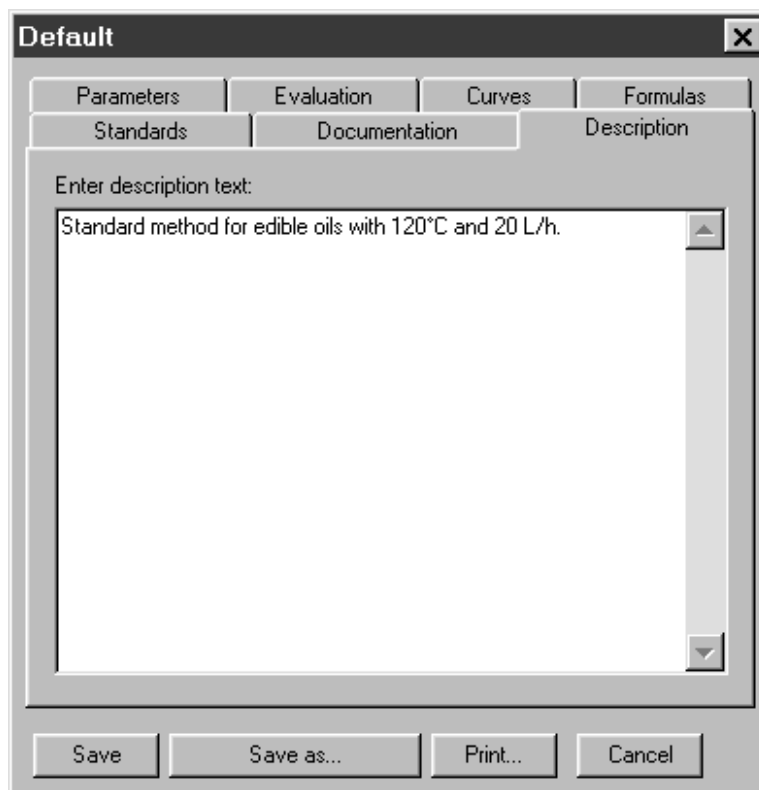



4.6 Determinations

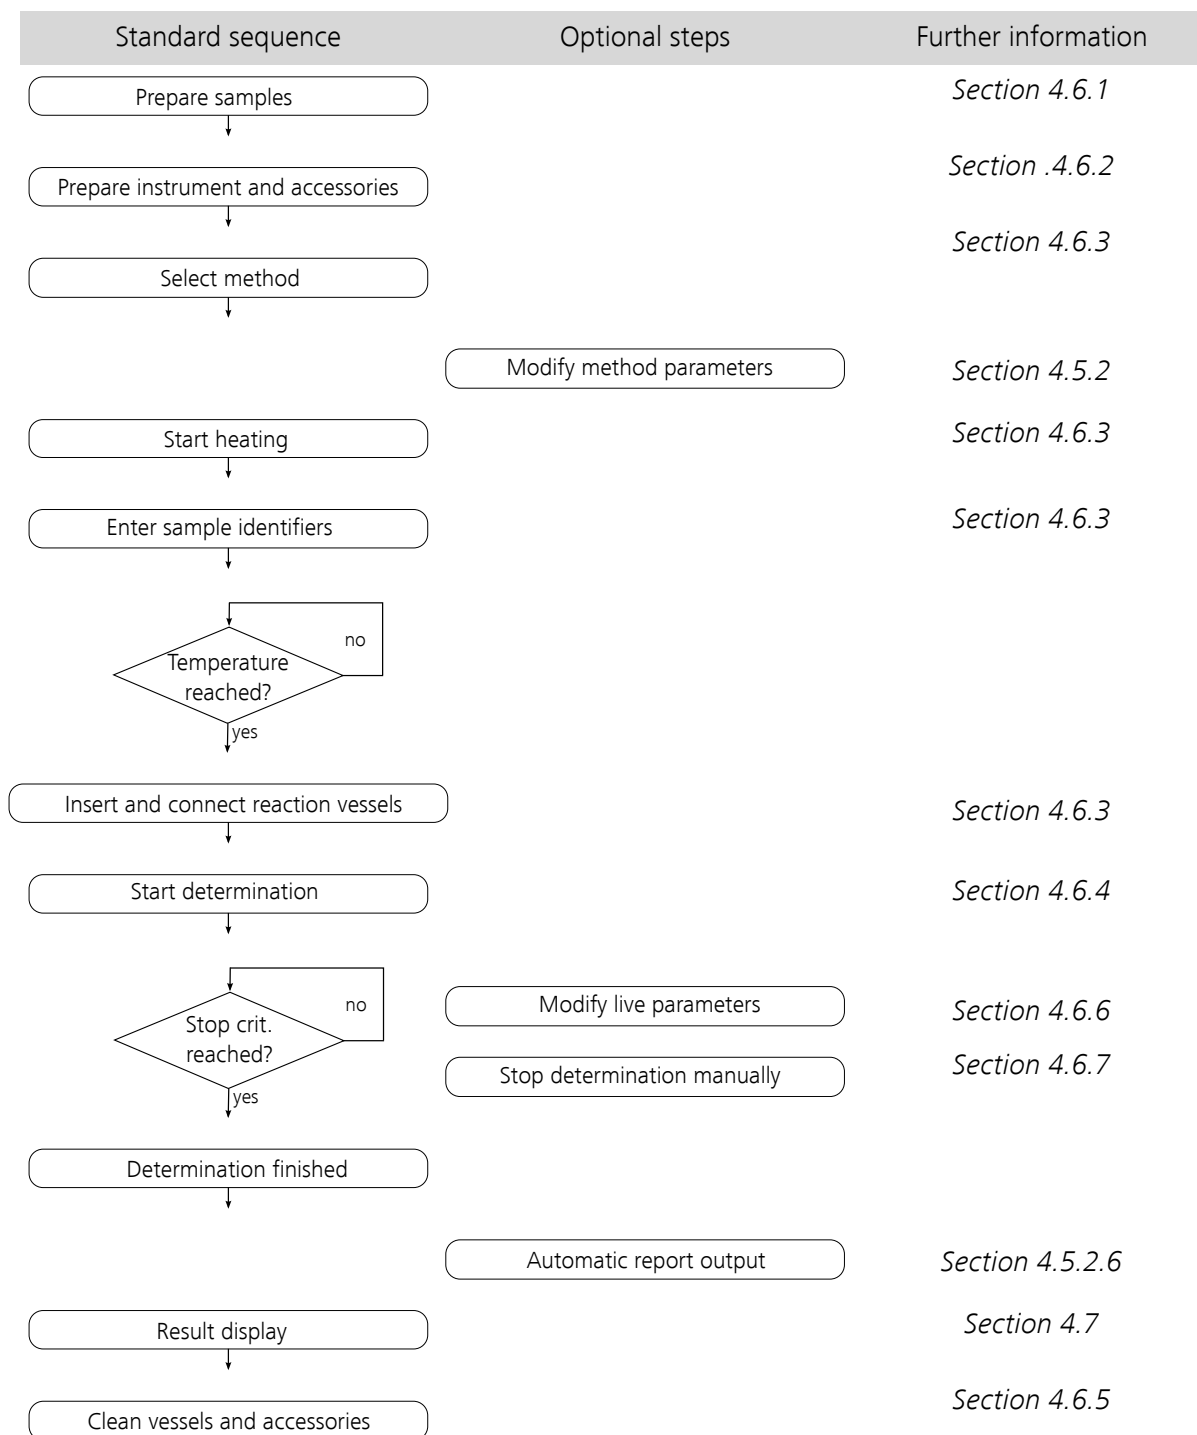

4.6.1 Preparing samples

This section contains information on how to prepare the following samples:

- Pure, clear oils (*see page 77*)
- Non-liquid, pure fats (*see page 77*)
- Samples containing oil and fat (*see page 78*)
- Emulsion fats (*see page 80*)



NOTICE

Use **new reaction vessels and air tubes** for each measurement. Blow the reaction vessel out with nitrogen before use.

Preparing pure, clear oil

Prepare the oil, which is completely pure and clear, as follows:

1 Weigh in the sample

- Weigh in **3 g sample material** directly in the reaction vessel.

2 Check the filling level

- Check whether the quantity of the sample material rises to such an extent in the reaction vessel that the air tube immerses sufficiently deeply. If this is not the case, add more sample material.

Preparing non-liquid, pure fats

Prepare non-liquid, pure fat as follows:

1 Weigh in the sample

either

- Completely **liquefy** the fat in a water bath or in a drying oven at a temperature exceeding its melting point by 10 °C.
- Then transfer **3 g sample material** using preheated pipettes to the reaction vessel.

or

- Weigh in the fat as **solid**. For this, weigh in **3 g sample material** directly in the reaction vessel and insert this briefly in the heated block of the 743 Rancimat, so that the fat melts.

**NOTICE**

If the folded filter becomes blocked (e.g. due to the consistency of the sample material), a Soxhlet apparatus should be used for solid/liquid separation. You can use up to 40 g of sample material here per approach.

3 Distillation and filtration

- Distill the petroleum ether from the clear, perhaps slightly yellow extract.

**NOTICE**

It is safest and easiest if you do this in a rotation evaporator; in a slight vacuum and at a temperature of +30...35 °C the petroleum ether can gently and efficiently be removed, protected from direct light (cover the water bath e.g. with aluminum foil).

- Dry the oil/fat sample obtained after completing the distillation: during around 30 min at a pressure of $p < 1330$ Pa (13.3 mbar).
- Filter the oil/fat sample now present together with **Na₂SO₄ water-free** over a folded filter. If necessary, work in the drying oven at a temperature exceeding the melting point of this fat by 10 °C.

4 Further sample preparation

- Treat the isolated oil/fat samples afterwards just as pure oils and fats.

**NOTICE**

If the isolated oil/fat samples are not immediately measured out, you have to store the samples **in a cool place and protected from light**; for storing the samples, they should be covered over in their vessels with a nitrogen layer. This type of storage does not provide complete protection against unintended and uncontrolled changes in the oxidation stability, but represents a usable preservation in many cases.

You can find further information on the treatment of oil and fat samples in **Rancidity in Foods**, Allen J.C., Hamilton R.J., *Applied Science Publishers*, London and New York, 1983.

Check and prepare the instruments and vessels as follows (see also figure 5, page 14):

1 Check openings for reaction vessels

- Check whether the openings are clean and empty. Blow the dust out of the openings with nitrogen.
If the instrument is not used, always seal the openings with the sealing plugs.

2 Fill the measuring vessels



NOTICE

Only use **measuring vessels** and accessories which are **absolutely clean** and in a **perfect condition**.

- Fill the cleaned measuring vessels with **60 mL distilled water** each.
For analysis times > 24 h approx. 7 mL more distilled water must be added per day to compensate for the evaporation loss, so that the electrodes remain safely immersed.

3 Insert the measuring vessels

- Place the clean measuring vessel covers equipped with a PTFE tube on the measuring vessels.
- Insert the measuring vessels with the measuring vessel covers into the openings provided for this on the 743 Rancimat and, at the same time, carefully guide the connection plugs (5-15) of the cover carefully into the electrode connectors (3-2).

4 Weigh in the sample



NOTICE

Use **new reaction vessels and air tubes** for each measurement. Blow the reaction vessels out with nitrogen before use so that any particles adhering are removed.

- Weigh in **3 g of the prepared samples** in each of the reaction vessels (see chapter 4.6.1, page 77).




5 Mount the accessories

- Take the upper edge of the reaction vessel in your hand (e.g. in the gap between your thumb and index finger) and turn the glass round once.
This serves for covering the degreased glasses with a light **fat film** so that the vessel covers can be removed more easily after the determination.
- Insert an air tube (5-5) in the connector (5-7) of the reaction vessel cover, fix it with the O-ring (5-6) and fasten it by screwing in the thread adapter M8 / M6 (5-3).
- Place the reaction vessel cover on the reaction vessel. Turn the cover in such a way that the air tube is as close as possible to the vessel wall.
- Connect the white silicone tubing to the tubing connector (5-4) of the reaction vessel cover.
- Place the prepared reaction vessel in the vessel holder.

4.6.3 Preparing the determination

1 Select method

- Under **Unit x Block A**, click on the symbol  in order to select the method for Block A.
- If required, also select a method for Block B.



NOTICE

Different methods with different temperatures can be selected for Block A and Block B. For the gas flow, on the other hand, the value which is defined in the method loaded for Block A applies for both blocks.

See also "*Opening a selected method and adjusting parameters*", page 58.

2 Start heating

- Under **Unit x Block A**, click on the button **[Heat to xx °C]**.
- If required, also switch on the heating for Block B.

The color of the button frame changes to red and the temperature display (2-3) on the instrument flashes. The current temperature is displayed directly next to the button.

Heating up duration for 120 °C: approx. 45 min.

Heating up duration for 200 °C: approx. 60 min.



NOTICE

If you wish to turn off the heating, click on the button **[Heat to xx °C]** again.

3 Enter sample identification

- Enter the sample identifications **ID1 & ID2** for all sample positions used.

ID1 & ID2	
Sunflower oil G5	▼
Sample 12793	

The entry for **ID1** can be selected from the automatically created list of already entered identifications. This list can be deleted again in the **Control window** with the menu item **Options ▶ Clear sample ID1 history**.

4 Insert and connect reaction vessels



NOTICE

The temperature defined in the method must be reached, before you insert the reaction vessels, i.e. the frame of the button **[Heat to xx °C]** must be **green**.

- Seal the channels not used with the sealing plugs or empty reaction vessels for protection against impurities.
- Insert the prepared reaction vessels into the openings of the heating block.
- Connect the white silicone tubings which are fastened to the reaction vessel cover to the tubing adapter M8 / olive (5-11) of the measuring vessel covers.
- Screw the FEP tubings 250 mm (5-1) to the thread adapters (5-3) of the reaction vessel covers and the air supply connections (3-3) of the Rancimat.

- Rinse the product thoroughly with distilled water.
- Clean the **measuring vessel covers (5-16)**, the **PTFE tubes (5-17)** and the **electrodes (5-18)** with acetone or 2-propanol and rinse with distilled water. Pre-clean with washing-up liquid in the case of severe contamination.
Remove the protective ring (5-19) to be able to clean the electrodes.

2 Clean the reaction vessels and accessories

- Dispose of used **reaction vessels** and **air tubes** and use new reaction vessels and air tubes for the next measurement.
- Clean the **reaction vessel covers** with acetone or 2-propanol and rinse with distilled water. Pre-clean with washing-up liquid in the case of severe contamination.
- Then heat the **reaction vessel covers** in the drying oven for 2 hours at 80 °C.



NOTICE

Replace the reaction vessel covers if they are not tightly on the reaction vessel anymore or the material is obdurate.

3 Clean the tubings

- Clean the **silicone tubings (5-2)** with acetone or 2-propanol and rinse with distilled water. Pre-clean with washing-up liquid in the case of severe contamination.
- Then heat the **silicone tubings** in the drying oven for 2 hours at 80 °C.

4.6.6 Adjusting the method parameters during the determination

1 Open the dialog window Live parameters

- In the **Control window**, click on the symbol  or the menu item **View ► Live parameters...**

The following dialog window appears:



2 Adjust the parameters

- Adjust all required parameters (see chapter 4.5.2.1, page 61).
- Confirm the changes with **[OK]**.

4.6.7 Stopping the determination manually

Determinations are normally automatically stopped after reaching the stop criteria defined in the method. Current determinations can also be stopped manually.

1 Stop determination

- In the **Control window**, click on the button **[Stop]**.


The message **Do you want to save this determination?** appears.

2 Save measured data and results

- Confirm the message with **[Yes]** to save all data of the determination.
- or confirm the message with **[No]** to reject all data.


4.6.8 Status of the live curve

Before a determination:



No active measurement.


The channel is ready for starting a determination.



No active measurement.


Communication error between instrument and PC.

During a determination:



Determination started.


The first measured value is measured.



Current measurement.

Measured value and time are displayed above the live curve.

After a determination:




Determination finished.


The channel is ready for starting a new determination.

A detailed description of the parameters can be found at "*Parameter description*", page 96.

1 Select fields

- Click on the symbol  or the menu item **Format ▶ Select fields**.

The following dialog window appears:

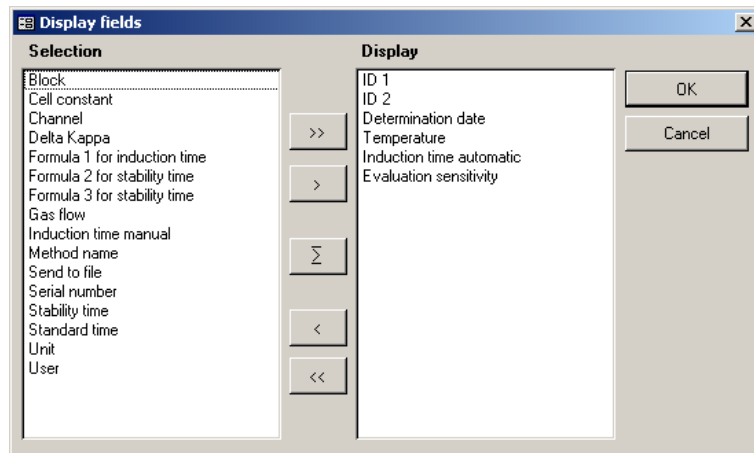


Only those fields are shown in the determination overview which are listed in the right column under **Display**.

- In the column **Selection**, click on a field which is to be displayed in the determination overview.
- Click on the [**>**] button.
- In the column **Display**, click on a field which is **not** to be displayed in the determination overview.
- Click on the [**<**] button.

2 Adjust the column width

- Click in any cell of the column whose width is to be adjusted.
- Click on the menu item **Format ▶ Adjust width**.

The following dialog window appears:

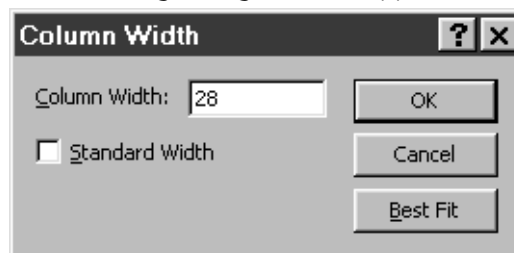


- Under **Column width**, enter the number of characters of a column and confirm with [**OK**].

or



- Position the cursor in the title line of the table between two columns.


The cursor assumes the following form: 

- Drag the column width to the required size keeping the left mouse button pressed down.

3 Adjust the cell format

- Click on the menu item **Format ► Fields....**

The following dialog window appears:

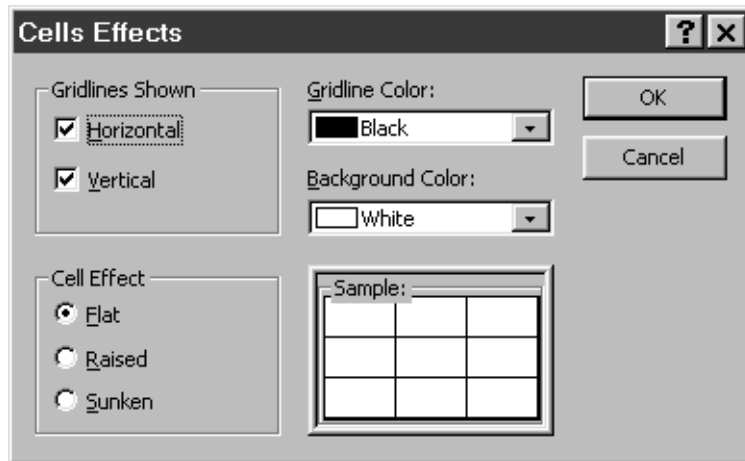

- Carry out the required settings and confirm with **[OK]**.

4 Change the font

- Click on the menu item **Format ► Fonts...**

The following dialog window appears:



- Carry out the required settings and confirm with **[OK]**.

Selecting determinations

Proceed as follows to select one or more lines of the determination overview:

1 Select a line

- Place the mouse button on the left edge of the line to be selected.
The cursor assumes the following form: ➔
- Click on the line.

2 Select several lines

- Place the mouse button on the left edge of the line to be selected.
The cursor assumes the following form: ➔
- Keep the mouse button pressed down and move over the left edge of all lines to be selected.



3 Select all lines

- Click on the menu item **Edit ▶ Select all records**.

or


- Click on the upper left in the title line.

Searching for determinations

Proceed as follows to search for specific determinations.

A detailed description of the parameters can be found at *"Find What"*, page 101.

1 Open search field

- Click on the symbol  or the menu item **Determination ▶ Find...**

The dialog window **Find in field: 'Field name'** appears.


2 Enter search criteria

- Enter the search term and the other search criteria.
- Click on the button **[Find first]** in order to search through the determination overview.


Sorting determinations

Proceed as follows to sort the columns of the determination overview:


1 Sort column ascending

- Click in the title line of the column to be sorted.
The entire column is highlighted in black.
- Click on the symbol  or the menu item **Determination ▶ Sort ▶ Ascending**.

2 Sort column descending

- Click in the title line of the column to be sorted.
The entire column is highlighted in black.
- Click on the symbol  or the menu item **Determination ▶ Sort ▶ Descending**.

3 Remove sorting again

- Click on the symbol  or the menu item **Determination ▶ Filter ▶ Remove filter/sorting**.


Displaying or hiding selected determinations

Proceed as follows to display or hide previously selected determinations only:


1 Select determinations

- See "*Selecting determinations*", page 91.

2 Display selected determinations only


- Click on the symbol  or the menu item **Determination ▶ Filter ▶ Filter selection**.

3 Remove the filter again

- Click on the symbol  or the menu item **Determination ▶ Filter ▶ Remove filter/sorting**.

All entries are once again displayed in the dialog window.


4 Hide selected determinations

- Click on the symbol  or the menu item **Determination ▶ Filter ▶ Selection not in filter**.

Filtering determinations with the "Selection based filter"

Proceed as follows to filter the entries of the determination overview according to a specific selection (cell or cell content):


1 Filter the entries

- Click in that cell which contains the required filter criterion (e.g. **Determination date** = "12.2005").
- Click on the symbol  or the menu item **Determination ▶ Filter ▶ Selection based filter**.

Only the entries with the **Determination date** "12.2005" are displayed in the dialog window.



2 Remove the filter again


- Click on the symbol  or the menu item **Determination ▶ Filter ▶ Remove filter/sorting**.

All entries are once again displayed in the dialog window.


Filtering determinations with the special filter

With a special filter you can define complex conditions for filtering and sorting data sets. In the following section, you will see a simple example of a special filter. You will find a detailed description of all parameters under "*BestimmungsübersichtFilter*", page 103.

1 Open dialog window

- Click on the symbol  or the menu item **Determination ▶ Filter ▶ Special filter/sorting...**

The following dialog window appears:

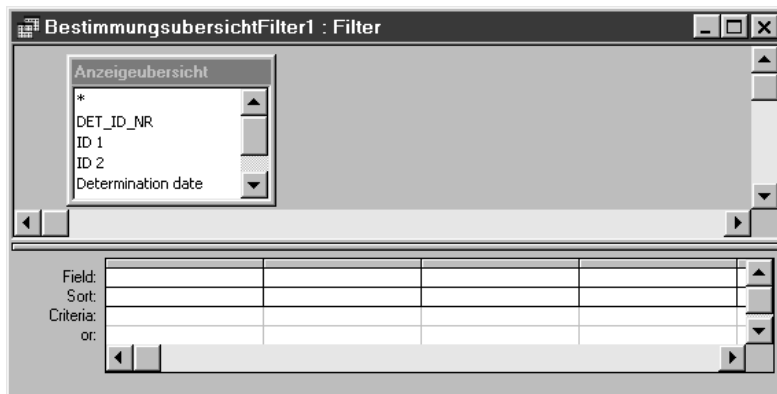

2 Select the fields which are to be filtered

- In the dialog window **Anzeigeübersicht**, double-click on the field **Determination date**.
- In the dialog window **Anzeigeübersicht**, double-click on the field **Temperature**.



NOTICE

In the dialog window **Anzeigeübersicht**, only those field are available for selection which are displayed in the determination overview (see "*Formatting the determination overview*", page 88).

The two fields are displayed in the lower part of the window under **Field:**

Field:	Determination date	Temperature
Sort:		
Criteria:		
or:		

3 Specify the filter criteria

- In the column **determination date** in field **Criteria** enter the value **05.04.2000*** (incl. asterisk as wildcard).
- In the column **Temperature** and the field **Criteria** enter the value **> 110**.



NOTICE

You will find a detailed description of the possible filter criteria under "*Criteria*", page 103.

4 Apply and remove the filter

- Click on the symbol or the menu item **Determination ▶ Filter ▶ Apply filter/sorting**.
In the window **Determination data**, all determination data is now displayed that was carried out on April 5, 2000 at a temperature of over 110 °C. In addition, the dialog window **Determination data** uses the word **FILTER** to indicate that the displayed data is filtered.
- Click on the symbol or the menu item **Determination ▶ Filter ▶ Remove filter/sorting**.
The special filter has been removed again.

Deleting determinations



NOTICE

Only the **Administrator** can delete determinations.



Proceed as follows to delete specific entries from the determination overview:

1 Select the determination

- See "Selecting determinations", page 91.


2 Delete the entry

- Click on the menu item **Determination ► Delete**.
The safety prompt **Do you really want to delete the selected determinations?** appears.
- Confirm the security query with **[Yes]**.

Printing and exporting the determination overview

See Chapter 4.7.6, Page 129.

Parameter description

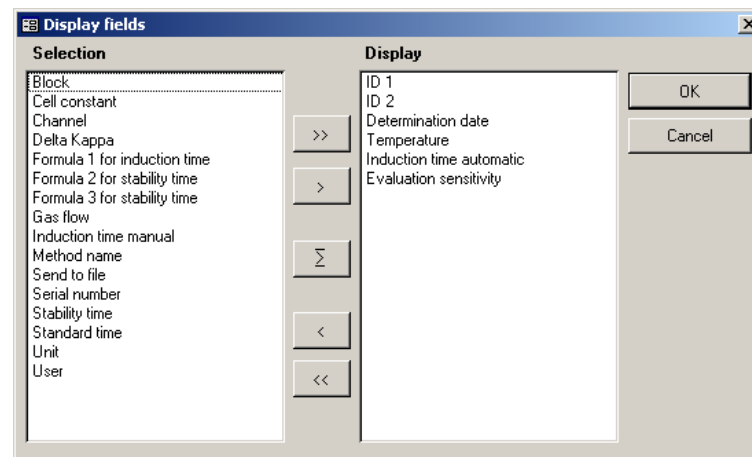

Selection

Selection of all fields, which can still be selected for the determination overview. The following **fields of the determination overview** are available:

Send to file

Directory in which the determination file (TXT file) has been saved.

Evaluation sensitivity

Evaluation sensitivity used for the determination of the induction time.

User

Name of the user who was logged in when recording the determination.

Determination date

Date and time at which the determination was started.

Block

Letter of the block used for the determination.

Delta Kappa

Conductivity change for the determination of the stability time.

Formula 1 for induction time

Result of the calculation with formula 1.

Formula 2 for stability time

Result of the calculation with formula 2.

Formula 3 for stability time

Result of the calculation with formula 3.

Gas flow

Gas flow through sample.

Unit

Number of the instrument used for the determination.

ID 1

Sample identification 1.

ID 2

Sample identification 2.

Induction time automatic

Automatically determined induction time.

Induction time manual

Induction time manually determined with the reevaluation.

Channel

Number of the channel used for the determination.

Method name

Name of the method with which the determination has been carried out.

Standard time

Automatically calculated standard time.



Serial number

Serial number of the instrument used to record the determination.

Stability time

Automatically or, with the reevaluation, manually determined stability time.

Temperature

Temperature as defined in the method.

Cell constant

Cell constant of the conductivity measuring cell used to record the determination.

Display

Fields which have been selected for the determination overview.

Selection	Fields of the determination overview
-----------	--------------------------------------



Move all fields in **Selection** to **Display**.



Move selected field in **Selection** to **Display**. The field is inserted at the end of the list.




Move selected field in **Selection** to **Display**. The field is inserted above the field selected in **Display**.



Move selected field in **Display** to **Selection**.



Move all fields in **Display** to **Selection**.

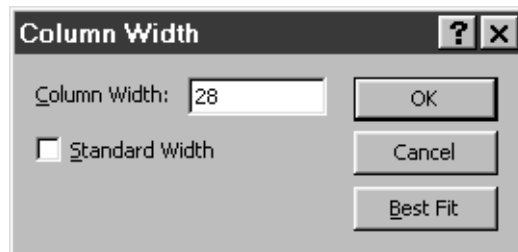



Column width

Width of the column in characters.

Entry	'Number of characters'
-------	-------------------------------


Standard width

on | off (Default value: **on**)

Reset the column width to standard width (18.5 characters).

[Best Fit]

Adjust the column width to the longest field content (including title).

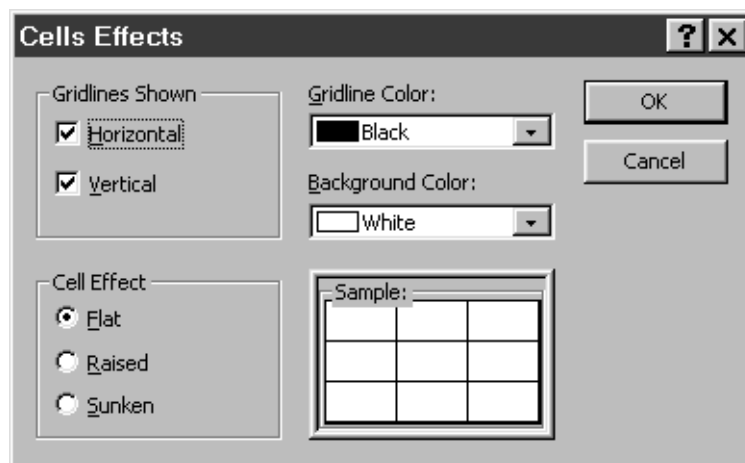

Gridlines Shown

Horizontal

on | off (Default value: **on**)

Display horizontal grid lines.

Vertical

on | off (Default value: **on**)

Display vertical grid lines.

Cell Effect

Selection	Flat Raised Sunken
-----------	-------------------------------

Flat

Flat view of the cells.

Raised

Raised view of the cells.

Sunken

Sunken view of the cells.

Selection **Color**

Font style

Choice of font style for the selected font type.

Selection **Standard | Italic | Bold | Bold italic**

Sample

Display of the selected font type.

Size

Font size in points for the selected font type.

Selection **Font size**



Find What

Required search term.

Entry **'Search term'**

The following characters can be used as wildcards:

*: any character sequence (e.g. *ab, *ab*, ab*)

?: single character (e.g. a?a, ??a, ab?)

#: single numeral (e.g. ##20, ab####, #23##)

Search

Search mode

Selection **All | Down | Up**

All

Search in the entire table.

Down

Search downwards as far as the table end.

Up

Search upwards as far as the table start.

Match

Search area where the entered text is to be searched for.

Selection **Whole field | Start of field | Any part of field**

Field

Selection of a field (column) from the determination overview.

Selection	Field from the determination overview
-----------	--

Sort

Sorting for the selected field.

Selection	Ascending Descending (not sorted)
-----------	--

Criteria

Criteria for filtering data sets.

or

Further criteria for filtering data sets.

In the lines **Criteria** and **or** and in all following lines, data sets can be filtered using expressions. An **expression** is a combination of operators, functions and field names for determining a condition for filtering data sets. In the following only the most important elements and rules are described and a few selected examples are given. For more extensive information please refer to the documentation on Microsoft Access.

*Operators, functions,
field names*

Mathematical operators +, -, =, *, /

Comparison operators <, >, <>, <=, >=, Between..., And...

Logical operators AND, OR, NOT

Wildcards * (any character string), ? (single character), # (single numeral)

Current date Date()

Current time Now() (date and time)

Other fields ["Field name"]

*Links with various
fields*

If conditions are specified in various fields, these conditions can also be linked with **AND** and **OR**. The following applies:

Criteria in the same line apply as AND conditions, i.e. only those data sets are displayed which satisfy all conditions.

Criteria in various lines apply as OR conditions, i.e. all data sets which fulfill one condition are displayed.

Examples

> 10 Values greater than 10.

oil All data with "oil" as part of the name.



2007	All data of the year 2007.
Between Date() And (Date) - 7)	All data of the previous week.

4.7.2 Determination and method data

For each determination you can view all the determination data (name, determination date etc.) and method data (name, parameters etc.) and print or export these.

A detailed description of the parameters can be found at "*Parameter description*", page 105.


Displaying determination and method data

Proceed as follows to display all determination and method data for a selected determination:

1 Display determination overview

- See "*Displaying the determination overview*", page 88.

2 Open dialog window

- Select the desired determination (see "*Selecting determinations*", page 91).
- In the Results window, click on the symbol  or the menu item **View ► Determination and method data**.

The dialog window **Determination and method data** appears.

Printing and exporting determination and method data

See Chapter 4.7.6, Page 129.

Parameter description

ID 1

Sample identification 1.

ID 2

Sample identification 2.

Determination date

Date and time at which the determination was started.

User

Name of the user logged in when recording the determination.

Serial number

Serial number of the instrument used to record the determination.

Cell constant

Cell constant of the conductivity measuring cell used to record the determination.

GLP test


GLP status at the time of recording the determination. The following displays are possible:

GLP test switched off: The GLP monitoring was not activated for either temperature or conductivity or gas flow.

GLP test due: The next GLP test was due.

GLP test not passed: The last GLP test carried out was not passed.

GLP test passed: The last GLP test carried out was passed.



Display of the instrument, block and channel on which the determination was carried out.

Determination and method data

Standards	Curves	Documentation	Warnings
Determination	Results	Method	Parameters
		Evaluation	Formulas
Induction time automatic	<input type="text" value="3.26"/>	h	
Induction time manual	<input type="text" value="0.00"/>	h	
Stability time	<input type="text" value="0.00"/>	h	
Delta Kappa	<input type="text" value="0"/>	μS/cm	
Formula 1 for induction time	<input type="text" value="0.00"/>	h	
Formula 2 for stability time	<input type="text" value="0.00"/>	h	
Formula 3 for stability time	<input type="text" value="0.00"/>	h	
Standard time	<input type="text" value="0.00"/>	h	

OK

Induction time automatic

Automatically determined induction time.

Induction time manual

Induction time manually determined with the reevaluation.

Stability time

Automatically or, with the reevaluation, manually determined stability time.

Delta Kappa

Conductivity change for the determination of the stability time.

Formula 1 for induction time

Result of the calculation with formula 1.

Formula 2 for stability time

Result of the calculation with formula 2.

Formula 3 for stability time

Result of the calculation with formula 3.

Standard time

Automatically calculated standard time.

The screenshot shows the 'Determination and method data' dialog box with the 'Method' tab selected. The 'Method name' is 'Oil 120°C', 'Creation date' is '20.02.2007', and 'Creator' is 'Administrator'. The 'Method description' field is empty. The 'OK' button is visible at the bottom right.

Method name

Name of the method.

Creation date

Date when the method was last saved.

Creator

Name of the logged in user who last saved the method.

Method description

Description of the method.

The screenshot shows the 'Determination and method data' dialog box with the 'Parameters' tab selected. The 'Temperature' is '120 °C', 'Delta T' is '1.40 °C', and 'Gas flow' is '20 L/h'. The 'Use internal pump' checkbox is checked. Under 'Start options', 'Start delay' is '0 min' and 'Start mode' is 'per channel'. Under 'Stop criteria', 'Endpoint' is checked. Under 'Switch-off at end of determinations', 'Gas flow' is checked. The 'OK' button is visible at the bottom right.

Temperature

Setpoint temperature of the sample.

**Delta T**

Temperature correction: indication of how much the block temperature has been increased so that the sample reaches the setpoint temperature.

Gas flow

Gas flow through sample.

Use internal pump

Gas supply with internal pump switched on/off.

Start options**Start delay**

Waiting time until starting the measurement.

Start mode

Mode for starting the channels:

per channel: all channels were started individually.

per 2 channels: 2 channels each have been started jointly.

per block: the 4 channels of a block were started jointly.

Stop criteria**Time**

Time until the automatic stop of the determination.

Conductivity

Conductivity limit value. The determination was automatically ended upon reaching this value.

Endpoint


Automatic stop of the determination, as soon as every endpoint (induction and stability time) has been reached.

Actions at end of determinations...**Shut off heater**

The heating was automatically deactivated at the end of the determination.

Shut off gas flow

The gas flow was automatically deactivated at the end of the determination.

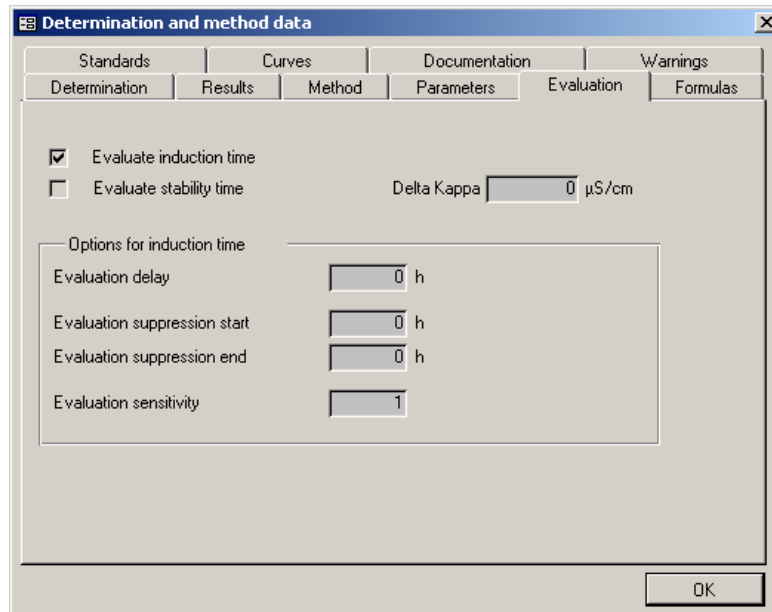

Evaluate induction time

The induction time has been automatically determined (see "Induction time", page 67).

Evaluate stability time

The stability time has been automatically determined (see "Stability time", page 68).

Delta Kappa

Conductivity change for the determination of the stability time.

Options for induction time

Evaluation delay

Waiting time until starting the curve evaluation.

Evaluation suppression

Start


Time from the start of the determination to the start of the evaluation suppression.

End

Time from the start of the determination to the end of the evaluation suppression.

Evaluation sensitivity

Evaluation sensitivity used for the determination of the induction time.

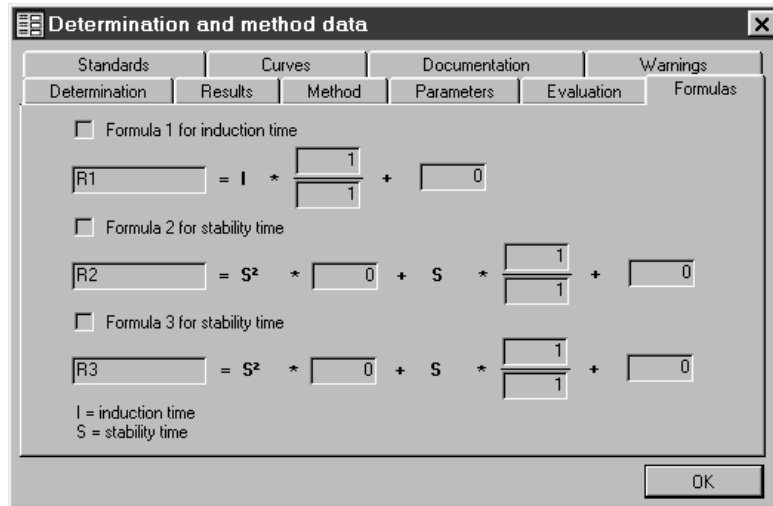

Formula 1 for induction time


The automatically determined induction time was calculated with these values and saved under the name shown in the field "R1".

Formula 2 for stability time

The automatically determined stability time was calculated with these values and saved under the name shown in the field "R2".

Formula 3 for stability time

The automatically determined stability time was calculated with these values and saved under the name shown in the field "R3".

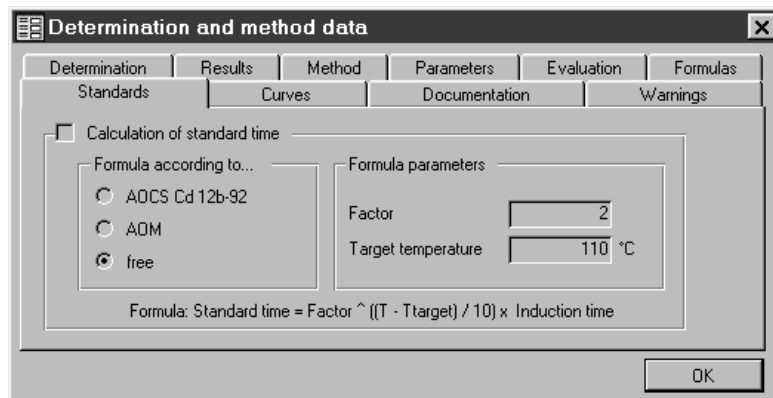

Calculation of standard time

Indicates whether the standard time has been calculated or not.

Formula according to...

AOCS Cd12b-92: Formula calculation according to standard AOCS Cd12b-92 with **Target temperature = 110 °C**.

AOM: Formula calculation according to standard AOM with **Target temperature = 97.8 °C**.

free: Formula calculation with freely selectable **Target temperature**.


Formula parameters

Factor

Parameter for the calculation of the standard time. It indicates by which factor the time changes per 10 °C.

Target temperature

Target temperature for the calculation of the standard time.

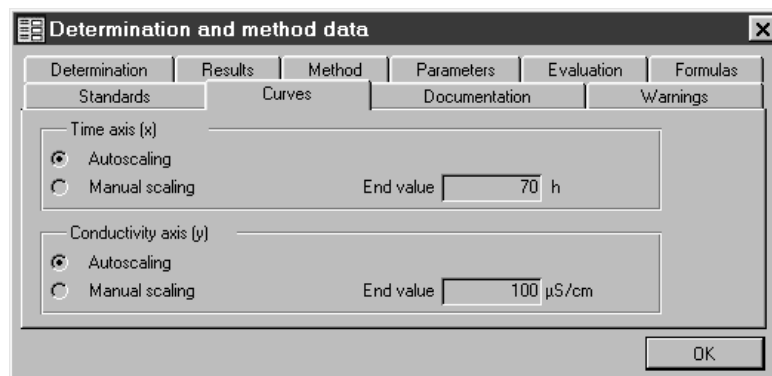

Time axis (x)

Autoscaling

Automatic definition of the start and end value of the time axis.

Manual scaling

Manual definition of the end value of the time axis.

End value

End value of the time axis with manual scaling.

Conductivity axis (y)

Autoscaling


Automatic definition of the start and end value of the conductivity axis.

Manual scaling

Manual definition of the end value of the conductivity axis.

End value

End value of the conductivity axis with manual scaling.

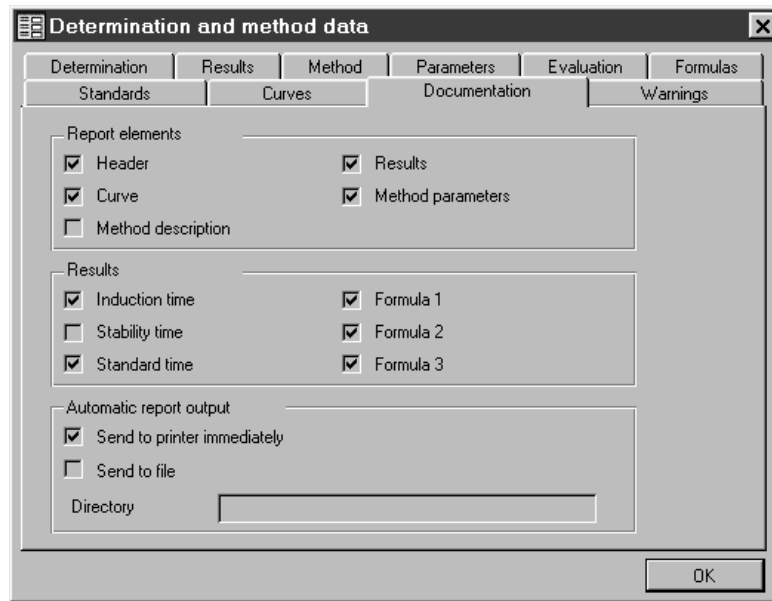

Report elements

Header

Output of the header.

Curve

Output of the curves.

Method description

Output of the method description entered on the tab **Description**.

Results

Output of the results selected below.

Method parameters

Output of the method parameters.

Results

Output of the selected results: **Induction time, Stability time, Standard time, Formula 1...3**.

Automatic report output

Send to printer immediately


Automatic printout of the report after finishing the determination.

Send to file

Automatic output of determination and method data after finishing the determination as a TXT file.

Directory

Directory in which the report has been saved.

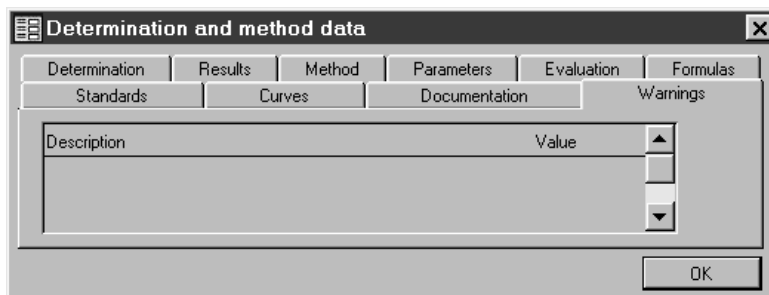

Description

The following warning messages are possible for incorrectly executed determinations:

Temperature not reached: setpoint temperature at start of the determination not reached.

Missing measuring points (start time): measuring points are missing from the given time (in s) onwards.

Missing measuring points (end time): measuring points are present again from the given time (in s) onwards.

Manual Stop: the determination was stopped manually with **[Stop]**.

Stop after communication error: Automatic stop of the determination because of interrupted connection between the Rancimat and the PC.

Value


Value for warning (e.g. temperature, time).

4.7.3 Graph and reevaluation

You can either open a graph of an individual determination (**single graph**) or have graphs of several determinations displayed above one another (**multiple graph**). In addition, you can open the so-called **live graph** of a determination, in the dialog window of which you can manually perform reevaluations of measuring curves.

You have the following options for reevaluation of graphs:

- Setting the induction time manually
- Setting the stability time manually
- Setting tangents manually

- Click on the symbol  or the menu item **Determination ► Graphics ► Live graph with reevaluation**.

The dialog window **Live graph** appears.

If present, the determined **induction time** (red, vertical line and numerical value) and **stability time** (black, vertical line and numerical value) are displayed in the graphics window next to the **measurement curve** (green).

With the button **[Evaluation]** you can display the second derivative of the measuring curve as well as the used evaluation sensitivity.

Zooming graphs, switching on/off offset and autoscaling

Proceed as follows to adjust the graph display:

1 Zoom graph

- See "Zooming", page 32.

2 Switch on/off offset for multiple curves

- Right click in the dialog window of a multiple graph. The context-sensitive menu for graphs appears.
- Click on the menu item **Offset**.

The offset for the displayed measurement curve is switched on or switched off.

In the case of an activated offset, the curves are arranged with an offset above one another. Instead of the usual lettering of the conductivity axis, the difference of the entire axis is in this case displayed in $\mu\text{S}/\text{cm}$.

3 Switch on/off autoscaling for single and live graphs

- Right click in the dialog window of a single graph or live graph. The context-sensitive menu for graphs appears.
- Click on the menu item **Autoscaling**.

The autoscaling for the displayed measurement curves is now activated or the manually performed scaling (see chapter 4.5.2.3, page 68) is canceled.

If this option is activated, the start and end values of the axes are automatically specified in such a way that all measured values are visible.

Setting the stability time manually



In order to set the stability time manually, you need to adjust the conductivity change **Delta Kappa**. After this, the stability time is recalculated automatically. Proceed as follows:

1 Open dialog window

- Right click in the dialog window of a live graph and click on the entry **Reevaluation** in the context-sensitive menu.

The dialog window **Reevaluation** appears.

2 Adjust Delta Kappa

- Click on the symbol .
- Under **Delta Kappa** enter the required value and confirm with the symbol .

The value of the calculated stability time is displayed both in the dialog window **Live graph** at the top right beside the gray line and also in the dialog window **Reevaluation** under **Stability time**.

3 Save changes

- In the dialog window **Live graph** click on the button **[Save]**.

The new stability time is accepted in the determination overview.

Setting tangents manually

For determining the **induction time**, you can manually set the tangents. The induction time is then defined as the **intersection of the tangents**. Set the tangents as follows:

1 Open dialog window

- Right click in the dialog window of a live graph and click on the entry **Reevaluation** in the context-sensitive menu.

The dialog window **Reevaluation** appears.

2 Set first tangent

- Click on the symbol .
- Keep the **[Ctrl]** key and **left mouse button pressed down** to set the first tangent.



3 Set second tangent

- Keep the **[Shift]** key and **left mouse button pressed down** to set the second tangent.

4 Adjust the position of the tangents

- Position the cursor on a black square on the tangent. The cursor assumes the form of a cross hair.
- Keep the **[Ctrl]** key and the **left mouse button pressed down** to move the point to the required position.

After you have adjusted the position of both tangents, you can read the value of the new induction time both in the dialog window **Live graph** at the top right beside the red line and also in the dialog window **Reevaluation** under **Manual**.


5 Save changes

- In the dialog window **Live graph** click on the button **[Save]**. The new induction time is accepted in the determination overview.

Deleting manually set tangents

Proceed as follows to delete the previously set tangents:

1 Delete tangents

- Click on the symbol .

Resetting all reevaluations

1 Reset induction and stability time to the original value

- Click on the **[Reset]** button.

4.7.4 Extrapolation

Extrapolation can be used to extrapolate the results measured at various temperatures to the required target temperature. In addition, the **factor** for converting the **induction time** to the **standard time** can be determined.

A detailed description of the parameters can be found at "*Parameter description*", page 121.

Extrapolation of several results

Proceed as follows to carry out an extrapolation of several results:


1 Open dialog window

- Open the Results window and the database (see "Displaying the determination overview", page 88).
- Select the required determinations (see "Selecting determinations", page 91).
- Click on the menu item **Determination ► Extrapolation**.

The dialog window **Extrapolation** with the extrapolation values which the program has calculated from the selected results (determinations) appears.

2 Select result and target temperature

- Click on the **[Settings]** button.
The following dialog window appears:

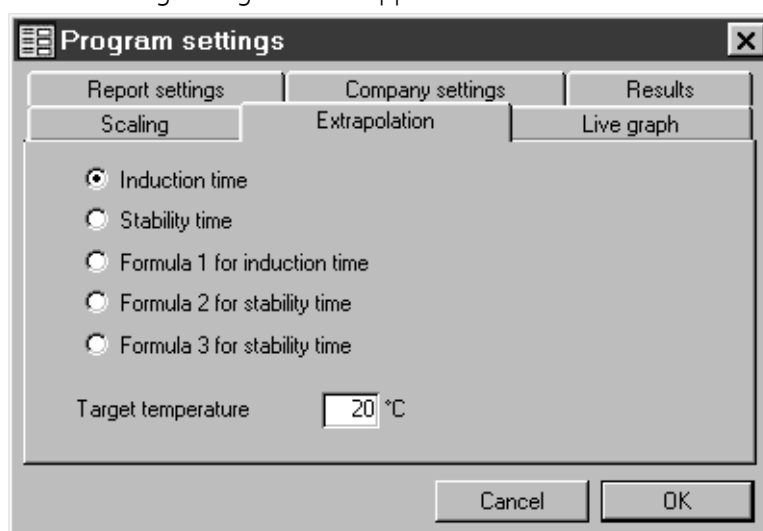

- Select the result which is to be used for extrapolation (**Induction time**, **Stability time**, etc.).
- Enter the **Target temperature**.
- Confirm the entries with **[OK]**.



NOTICE

The time determined for a particular sample by extrapolation to low target temperatures (e.g. 25 °C) is a purely theoretical value. The interrelation between this time and e.g. the perishability of the sample must be determined experimentally.



3 Update the display

- Click on the **[Update]** button.

The graph and all results are updated.



NOTICE

For extrapolation of the induction times, the manually changed values of the selected determinations (if present) are used, otherwise the automatically determined values are used.

Setting the correlation limit




NOTICE

The correlation limit for the **correlation coefficient r^2** can only be set by an Administrator.

1 Open dialog window

- In the Results window, click on the menu item **Options ▶ Administrator ▶ Extrapolation parameter**.

The following dialog window appears:

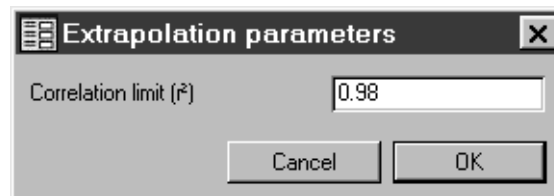

2 Adjust limit

- Under **correlation limit (r^2)** enter a value between 0 and 1 and confirm with **[OK]**.


Copying a graph and pasting it into other programs

See "Copying graphs and pasting them into other programs", page 116.

Printing extrapolation results

See "Printing extrapolation results", page 133.

Parameter description

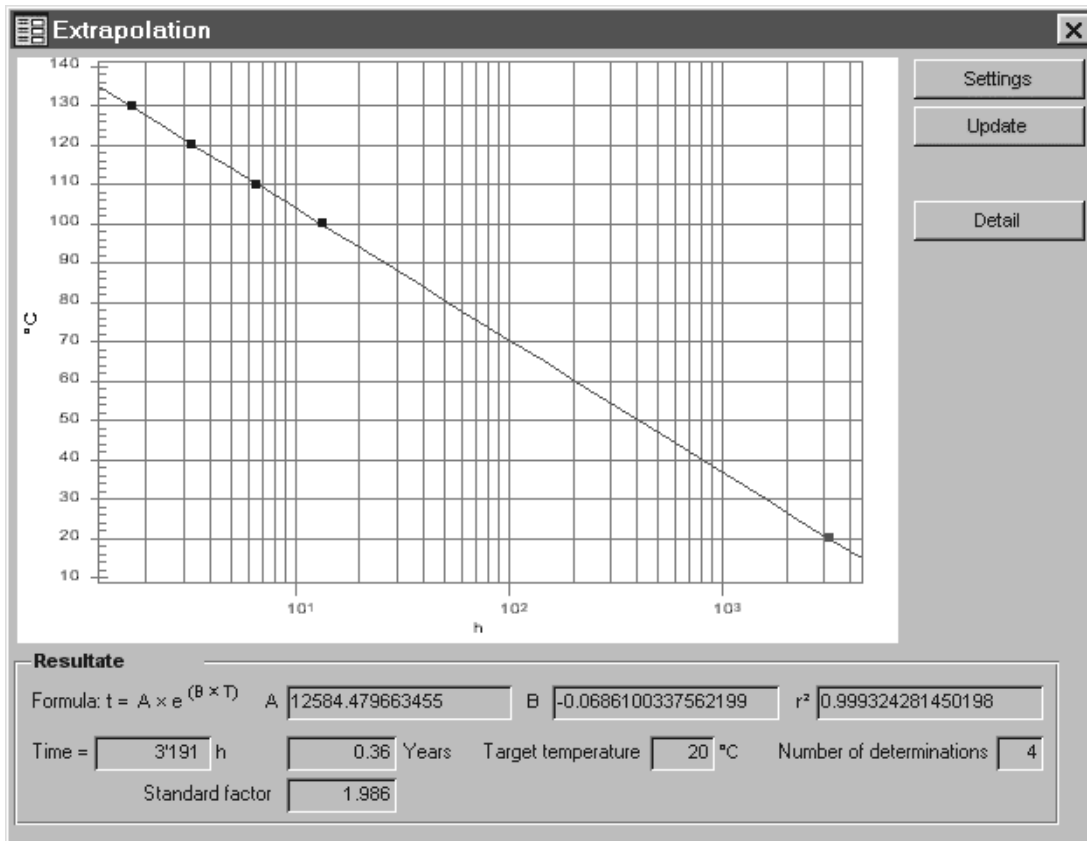

In the graphic **temperature vs. time** the linear regression is used to represent the calculated straight line $T = \ln(t)/B - \ln(A)/B$. The measured values of the selected determination are shown in **black**, the regression line in **green** and the time calculated for the target temperature in **red**.

Results

Formula

Exponential formula for calculating the time extrapolated from the measured values for the target temperature.

A

Calculated coefficient A of the exponential formula.

B

Calculated coefficient B of the exponential formula.

r^2

Calculated correlation coefficient. If this value is below the limit value (see "Setting the correlation limit", page 120) specified by the administrator a warning appears when opening the extrapolation window.

**Time**

Result of the extrapolation for the target temperature in hours and years.

Target temperature

Target temperature for the extrapolation.

Number of determinations

Number of determinations used for the extrapolation.

Standard factor

Value determined from the regression straight line which indicates the factor by which the time changes per 10 °C. This value can be entered in the formula for the determination of the standard time as a factor (see "*Calculation of standard time*", page 110).

[Settings]

Open the dialog window **Program settings**. The extrapolation parameters are to be entered in the tab **Extrapolation** (see "*Extrapolation*" tab", page 140).

[Update]

Update graphics and result display. This function has to be carried out if the selection of determinations in the determination overview or the settings for the extrapolation have been changed.

[Detail]

Display only the area with the results of the determinations in the graph.

4.7.5 Recalculating a determination

For a determination, you can recalculate the **Induction time**, the **Stability time**, the **Formulas** and the **Standard time**.

Recalculating the induction time

Proceed as follows to recalculate the induction time:

1 Open dialog window

- Select the determination which is to be recalculated (see "*Selecting determinations*", page 91).
- Click on the menu item **Determination ► Recalculation**.

The dialog window **Recalculation** appears.

2 Adjust the parameters

- Activate the options **Recalculate induction time** and **Calculation active**.
- Under **Evaluation delay** and **Evaluation suppression start/end**, enter the required values.
- Under **Evaluation sensitivity**, enter the required value.
The software suggests a value with which the highest maximum of the second derivative is accepted as the induction time. If there is no suggestion then the highest maximum has already been accepted.
The default value "1" will lead to the correct result for most applications. Smaller values will cause the acceptance of smaller maximums of the second derivative. Higher values require a higher maximum.
- Confirm the entries with **[OK]**.



NOTICE

A detailed description of the parameters can be found at "*Recalculate induction time*", page 125.

Recalculating the stability time

Proceed as follows to recalculate the stability time:

1 Open dialog window

- Select the determination which is to be recalculated (see "*Selecting determinations*", page 91).
- Click on the menu item **Determination ► Recalculation**.

The dialog window **Recalculation** appears.

2 Adjust the parameters

- Activate the options **Recalculate stability time** and **Calculation active**.
- Under **Delta Kappa** enter the required value and confirm with **[OK]**.



NOTICE

A detailed description of the parameters can be found at "*Recalculate stability time*", page 126.

- Under **Formula according to...** and **Formula parameters**, enter the required values and confirm with **[OK]**.



NOTICE

A detailed description of the parameters can be found at "Recalculate standard time", page 128.

Parameter description

Recalculate induction time

on | **off** (Default value: **off**)

Activate/Deactivate recalculation of the induction time. If the recalculation is deactivated, the original result is kept.

Calculation active

on | **off** (Default value: **on**)

If this option is **activated**, the parameters can be re-entered for the calculation of the induction time.

If this option is **deactivated**, the original result is deleted.

Evaluation delay

Waiting time until starting the curve evaluation.

**Evaluation suppression start**

Time from the start of the determination to the start of the evaluation suppression.

Evaluation suppression end

Time from the start of the determination to the end of the evaluation suppression.

Evaluation sensitivity

This value defines the minimum value which the maximum of the curve of the second derivative has to reach in order to be accepted as a result. The result, i.e. the induction time, is the time until the first accepted maximum.

The default value "**1**" will lead to the correct result for most applications. Smaller values will cause the acceptance of smaller maximums of the second derivative. Higher values require a higher maximum.

The software suggests a value with which the highest maximum of the second derivative is accepted as the induction time. If there is no suggestion then the highest maximum has already been accepted.

Recalculate stability time

on | off (Default value: **off**)

Activate/Deactivate recalculation of the stability time. If the recalculation is deactivated, the original result is kept.

Calculation active

on | off (Default value: **off**)

If this option is **activated**, **Delta Kappa** can be re-entered for the calculation of the stability time.

If this option is **deactivated**, the original result is deleted.

Delta Kappa

Conductivity change for the determination of the stability time in $\mu\text{S}/\text{cm}$.

Recalculation

Method Formulas Standards

Recalculate formula 1 for induction time

Calculation active

R1 = I * $\frac{1}{1}$ + 0

Recalculate formula 2 for stability time

Calculation active

R2 = S² * 0 + S * $\frac{1}{1}$ + 0

Recalculate formula 3 for stability time

Calculation active

R3 = S² * 0 + S * $\frac{1}{1}$ + 0

I = induction time
S = stability time

Cancel OK

Recalculate formula 1 for induction time

on | off (Default value: **off**)

Activate/Deactivate the recalculation of the result calculated with formula 1. If the recalculation is deactivated, the original result is kept.

Calculation active

on | off (Default value: **off**)

If this option is **activated**, the parameters for formula 1 can be re-entered.

If this option is **deactivated**, the original result is deleted.

Recalculate formula 2 for stability time

on | off (Default value: **off**)

Activate/Deactivate the recalculation of the result calculated with formula 2. If the recalculation is deactivated, the original result is kept.

Calculation active

on | off (Default value: **off**)

If this option is **activated**, the parameters for formula 2 can be re-entered.

If this option is **deactivated**, the original result is deleted.

AOCS Cd12b-92

Formula calculation according to standard AOCS Cd12b-92 with **Target temperature = 110 °C**.

AOM

Formula calculation according to standard AOM with **Target temperature = 97.8 °C**.

free

Formula calculation with freely selectable **Target temperature**.

Formula parameters**Factor**

Parameter for the calculation of the standard time, which indicates the factor by which the time changes per 10 °C.


Target temperature

Target temperature for the calculation of the standard time.


4.7.6 Printing and exporting data**Printing results from the Control window**

Proceed as follows to print results of the completed determinations shown in the Control window:

1 Open dialog window

- In the **Control window**, click on the symbol  or the menu item **File ► Print...**

The following dialog window appears:

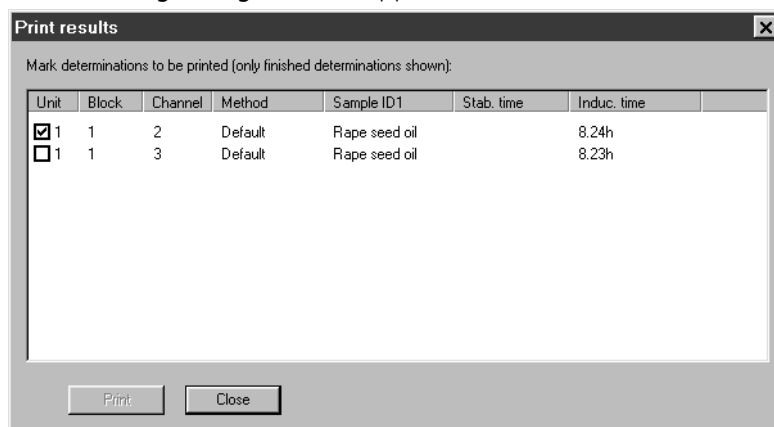**2 Print results**

- If required, adjust the column width (see "Formatting the determination overview", page 88).



- Select the required determinations and click on **[Print]**.

The results are printed according to the settings which have been defined in the method on the tab **Documentation**.


Printing determination overview

You can print a determination overview either in the form of a table or a list. Proceed as follows:

1 Display determination overview

- See *"Displaying the determination overview"*, page 88.

2 Select type of output (table or list)

- Click on the symbol  or the menu item **File ► Print...**.
The dialog window **Printing of...** appears.
- Click on the option **Overview table** and/or **Overview list**.



NOTICE

In the overview table, only those columns are printed which are within the maximum print width (15 cm).

3 Print determination overview

- Click on the **[Print]** button.
The dialog window **Print** appears.
- Select the required printer and click on **[Print]**.

The determination overview will be printed.

Printing determination and method data

Proceed as follows to print the determination and method data of one or several determinations:


1 Display determination overview

- See *"Displaying the determination overview"*, page 88.

2 Select determination

- Select the determination of which the data is to be printed (see *"Selecting determinations"*, page 91).

3 Select data

- Click on the symbol  or the menu item **File ▶ Print...**. The dialog window **Printing of...** appears.
- Select the option **All determination and method data** and confirm with **[Print]**.

The dialog window **Print** appears.

4 Print data

- Select the required printer and click on **[Print]**.

The determination and method data will be printed.


Printing graphs

Proceed as follows to print a single graph, multiple graph or live graph:

1 Open graph

- See "*Single graph, multiple graph or live graph*", page 114.

2 Print graph

- Click on the symbol  or the menu item **File ▶ Print...**. The dialog window **Print** appears.
- Select the required printer and click on **[Print]**.

The graph will be printed.

Printing the report defined in the method

Proceed as follows to print the report of one or several determinations, which has been defined in the method (see chapter 4.5.2.6, page 72):


1 Display determination overview

- See "*Displaying the determination overview*", page 88.

2 Select determination

- Select the determination of which the report is to be printed (see "*Selecting determinations*", page 91).

3 Select data

- Click on the symbol  or the menu item **File ▶ Print...**. The dialog window **Printing of...** appears.



- Select the option **Determination according to method** and confirm with **[Print]**.

The dialog window **Print** appears.

4 Print report

- Select the required printer and click on **[Print]**.

The report will be printed.

Printing the report defined under "Settings"

Proceed as follows to print the report of one or several determinations, which has been defined under **Settings**:


1 Display determination overview

- See "*Displaying the determination overview*", page 88.

2 Select determination

- Select the determination of which the report is to be printed (see "*Selecting determinations*", page 91).

3 Select data

- Click on the symbol  or the menu item **File ▶ Print...**
The dialog window **Printing of...** appears.
- Select the option **Determination according to settings**.

4 Carry out settings

- Click on the **[Settings]** button.
The dialog window **Program settings** appears.
- Carry out the required settings (see tab "*Report settings*", page 137) and confirm with **[OK]**.

The dialog window **Printing of...** appears.

5 Print report

- Click on the **[Print]** button.
The dialog window **Print** appears.
- Select the required printer and click on **[Print]**.

The report will be printed.


Printing extrapolation results

Proceed as follows to print the **extrapolation graph** (normal and detailed view), the **extrapolation results** and the overview of the **determinations** used for the extrapolation with the fields ID 1, ID 2, temperature and result:

1 Display extrapolation results

- See "Extrapolation of several results", page 119.

2 Print extrapolation results

- Click on the symbol  or the menu item **File ▶ Print...**
The dialog window **Print** appears.
- Select the required printer and click on **[Print]**.

The extrapolation results will be printed.

Exporting the determination overview to Word or Excel

Proceed as follows to export the determination overview to Word or Excel:


1 Select determinations

- See "Selecting determinations", page 91.
If you do not select any determinations, the entire overview is exported.

2 Select export program

- Click on the symbol  or the menu item **Determination ▶ Export ▶ Export to MS Word**.
The data is copied to a RTF file to be opened automatically by Microsoft Word.

or

- Click on the symbol  or the menu item **Determination ▶ Export ▶ Export to MS Excel**.
Microsoft Excel will be opened automatically.



Exporting determination and method data to a TXT file

Proceed as follows to export the determination and method data of one or several determinations to a TXT file:


1 Display determination overview

- See *"Displaying the determination overview"*, page 88.

2 Select determination

- Select the determination of which the data is to be exported (see *"Selecting determinations"*, page 91).

3 Export data

- Click on the symbol  or the menu item **Determination ► Export ► Determination and method data**.
The dialog window **Save to export file** appears.
- Select memory location, enter file name and confirm with **[Save]**.

The determination and method data will be exported.

Exporting determinations to another database

You can export determinations from a database to another existing database or a newly created database. Proceed as follows:

1 Display determination overview

- See *"Displaying the determination overview"*, page 88.


2 Select determination

- Select the determination to be exported (see *"Selecting determinations"*, page 91).

3 Select database

- Click on the menu item **Determination ► Export ► Export to database**.
The dialog window **Export data to...** appears.
- Select an existing database.
or
Under **File name** enter the name for the new database.
- Confirm the selection or entry with **[Save]**.

The following message appears (only for the Administrator):

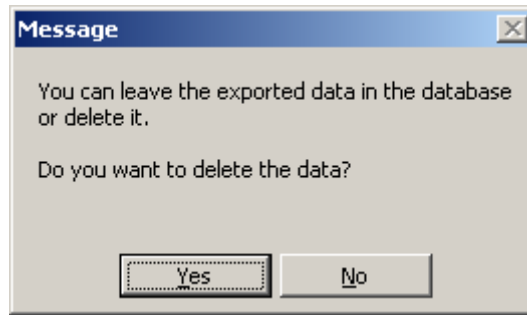

4 Keep or delete determination

- Click on **[No]** to also **keep** the exported determination in the original database.
- Click on **[Yes]** to **delete** the exported determination in the original database.

Opening the database in Microsoft Access 97




NOTICE

Each database is password-protected. The password is generated automatically by the program and can only be read by the Administrator.

The databases are saved in the installation directory of the 743 Rancimat program at **C:\Program Files\Metrohm\Rancimat\Database**.

1 Open Results window

- In the **Control window**, click on the symbol  or the menu item **File ▶ Results....**

The **Results window** appears.

2 Read out database password

- In the **Results window**, click on the menu item **Options ▶ Administrator ▶ Database password**. The dialog window **Open** appears.
- Select the required database and confirm with **[Open]**.

The dialog window **Password** appears with the password for the previously selected database.

3 Open database in Microsoft Access 97

- Start Microsoft Access 97.



- Open the required database by entering the previously read out password.

Exporting the measured value list

Proceed as follows to export a list of all measured values to a TXT file:


1 Display determination overview

- See *"Displaying the determination overview"*, page 88.

2 Select determination

- Select the determination of which the data is to be exported (see *"Selecting determinations"*, page 91).

3 Export data

- Click on the symbol  or the menu item **Determination ▶ Export ▶ List of measured values**.
The dialog window **Save to export file** appears.
- Select the memory location, enter the file name and confirm with **[Save]**.

The measured values list will be exported.

4.7.7 Program settings

Carrying out settings for the representation and output of results

You can carry out settings for the representation and output of results as follows:

1 Open dialog window

- In the **Results window**, click on the menu item **Options ▶ Settings**.


2 Carry out settings

- See the following *"Report settings" tab*.

4.7.7.1 Parameter description

"Report settings" tab

On the **Report settings** tab, you can carry out the settings for the report output.

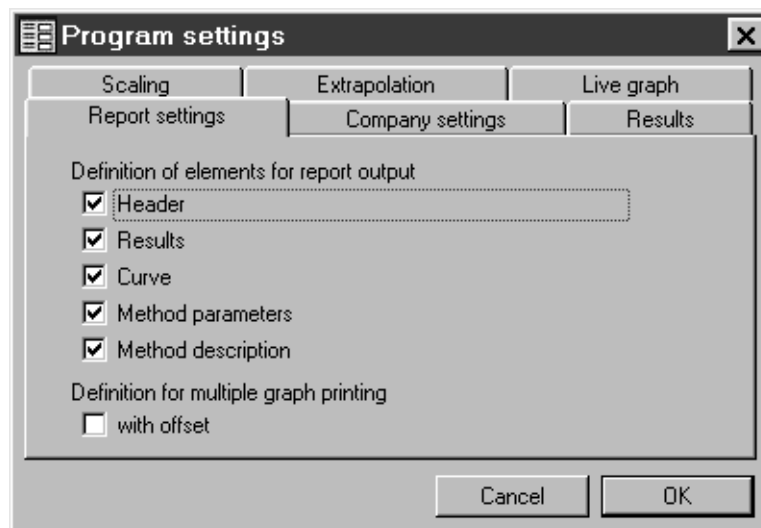

Definition of elements for report output

Header

on | off (Default value: **on**)

Output of the header with company settings (if defined, *see "Company settings" tab*), date of the printout, sample identifications, instrument information, determination date, user, cell constant and serial number.

Results

on | off (Default value: **on**)

Output of the results selected in the **Results** tab (*see page 139*).

Curve

on | off (Default value: **on**)

Output of the curves.

Method parameters

on | off (Default value: **on**)

Output of the method parameters.



Method description

on | off (Default value: **on**)

Output of the method description entered in the tab **Description**.

Definition for multiple graph printing


with offset

on | off (Default value: **off**)

If this option is activated, the curves are arranged with an offset above one another in the case of an output of multiple graphs. Instead of the usual lettering of the conductivity axis, the difference of the entire axis is, in this case, printed in $\mu\text{S}/\text{cm}$.

"Company settings" tab

On the **Company settings** tab, you can carry out the settings for the output of company logo and company text in the header.

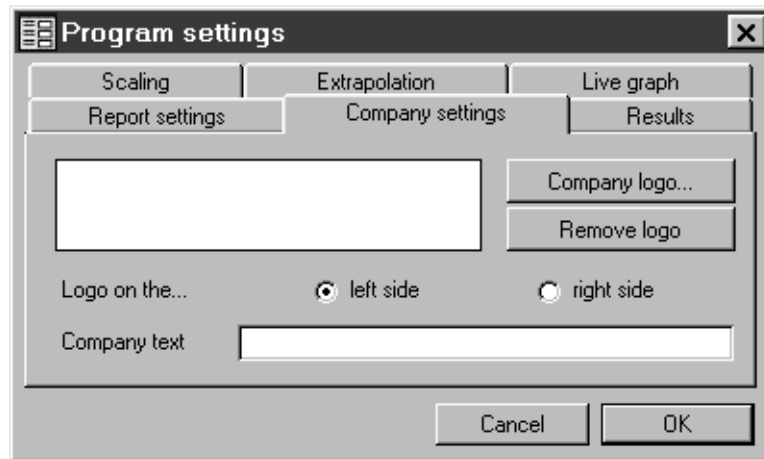

[Company-logo...]

Open the window **Find company logo** for selecting the graphics file with the company logo. Only WMF or BMP files can be used. After clicking on **[Open]**, the logo is displayed in the adjoining window.

[Remove logo]

Remove the embedded company logo.

Logo on the...

Selection	left side right side
-----------	-------------------------------

left side

The company logo is printed out on the left edge of the header.

right side

The company logo is printed out on the right edge of the header.


Company text

The text entered here is printed out on the side of the header opposite the company logo.

Entry	Characters
-------	-------------------

"Results" tab

On the **Results** tab, you can carry out the settings for the result output.

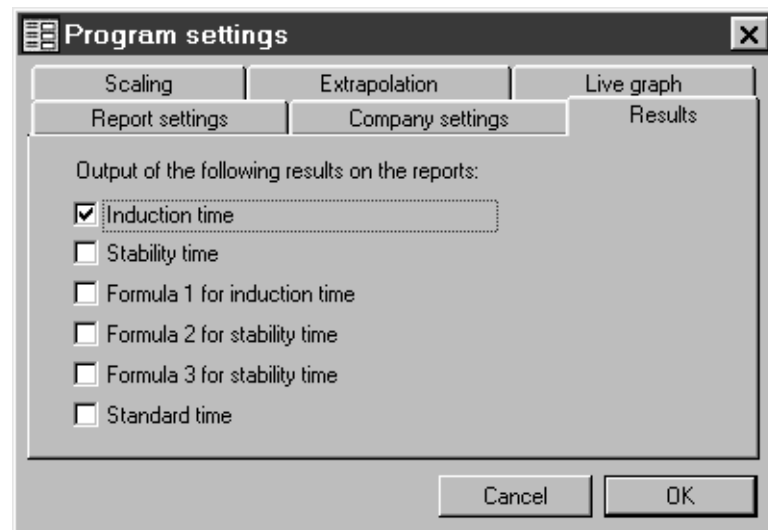

Output of the following results on the reports:

Induction time

on | **off** (Default value: **on**)

Stability time

on | **off** (Default value: **off**)

Formula 1 for induction time

on | **off** (Default value: **off**)

Formula 2 for stability time

on | **off** (Default value: **off**)

Formula 3 for stability time

on | **off** (Default value: **off**)


Standard time

on | **off** (Default value: **off**)



"Scaling" tab

On the **Scaling** tab, you can carry out the settings for scaling the curve axes.

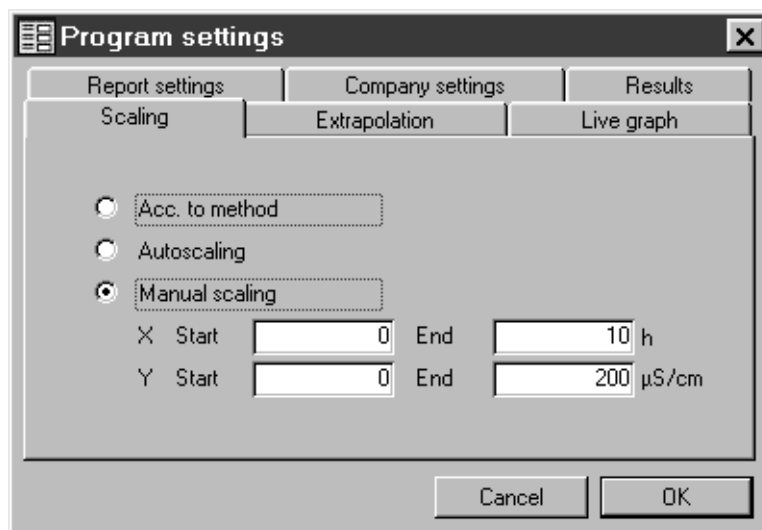

Acc. to method

Axis scaling in accordance with the settings defined in the method under **Curve representation** (see chapter 4.5.2.3, page 68).

Autoscaling

Automatic definition of the start and end values of the curve axes.

Manual scaling

Manual definition of the start and end values of the curve axes.

X Start

Start value of the time axis in hours.

X End

End value of the time axis in hours.

Y Start


Start value of the conductivity axis in $\mu\text{S}/\text{cm}$.

Y End

End value of the conductivity axis in $\mu\text{S}/\text{cm}$.

"Extrapolation" tab

On the **Extrapolation** tab, you can carry out the settings for the extrapolation.

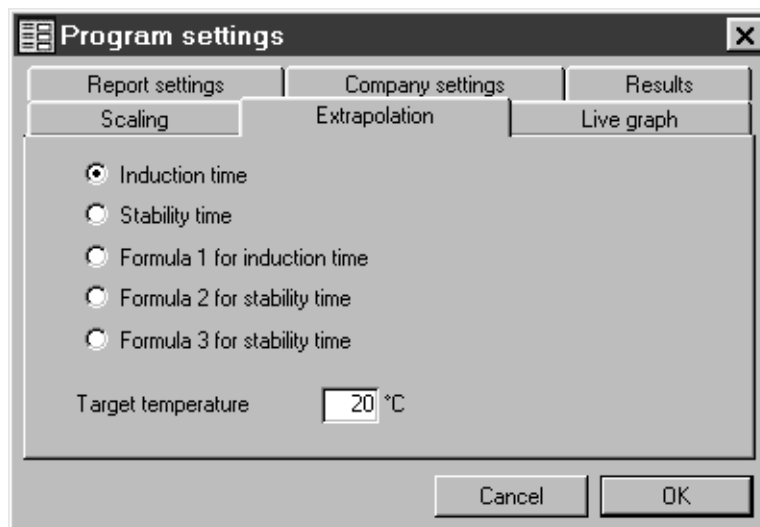

Induction time

The induction time is used for extrapolation. If the induction time has been determined manually, this value will be used and not the automatically determined induction time.

Stability time

The stability time is used for extrapolation.

Formula 1 for induction time

The result calculated with formula 1 is used for extrapolation.

Formula 2 for stability time

The result calculated with formula 2 is used for extrapolation.

Formula 3 for stability time

The result calculated with formula 3 is used for extrapolation.


Target temperature

Temperature, for which the selected result is to be converted. The conversion is realized using the regression straight line (from the extrapolation).

Input range **freely selectable - °C**

"Live graph" tab

On the **Live graph** tab, you can carry out the settings for displaying the live graph.

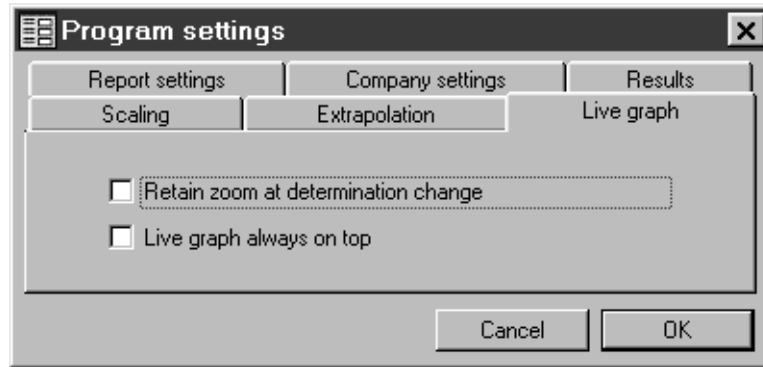

Retain zoom at determination change

on | off (Default value: **off**)

The selected zoom range is retained when changing the determination in the determination overview.

Live graph always on top

on | off (Default value: **off**)

The **Live graph** window is always displayed in the foreground.

4.7.8 Arranging windows

In the Results window, you can arrange the opened dialog windows either **above one another**, **beside one another** or **overlapping**. Proceed as follows:

1 Open windows

- Open all required dialog windows.
The following dialog windows can be opened in the Results window:
 - Determination overview (**View ▶ Determination overview**)
 - Graphs (**Determination ▶ Graphics ▶ Single/Multiple/Live graph**)
 - GLP window (**View ▶ GLP**)

2 Arrange windows

- Click on the menu item **Window ▶ Tile vertically** or **Window ▶ Tile horizontally** or **Window ▶ Cascade**.

The opened dialog windows are correspondingly arranged.

4.8 GLP functions

4.8.1 General information on GLP and validation

GLP (Good Laboratory Practice) requires, amongst other things, the periodical testing of analytical measuring devices for their reproducibility and correctness on the basis of **Standard Operating Procedures (SOP)**.

An example of such a standard operating procedure for the 743 Rancimat is available from Metrohm under the title *Application Bulletin No. 278 – Validation of Metrohm Rancimats*.

The operating software for the 743 Rancimat contains prepared **GLP tests** for temperature, conductivity and gas flow measurement. The user can determine whether and which tests have to be carried out. In addition, the time interval between the tests and the accuracy requirements can be specified. If the GLP function is activated, each results report receives a comment whether the GLP tests are fulfilled. Metrohm offers a GLP test set to carry out these tests .

Further information on the subject of QA, GLP and validation can also be found in the brochure *Quality Management with Metrohm* available from your Metrohm representative.

Electronic and mechanical functional groups in Metrohm instruments can and should be checked as part of regular service by specialist personnel of the manufacturing company. All Metrohm instruments are provided with start-up test routines which check the perfect functioning of the relevant assemblies when switching on the instrument. If no error message is displayed, it can be assumed that the instrument functions without fault.

The 743 Rancimat also contains an integrated diagnostic program which enables the service technician to check certain assemblies if any faults or incorrect functioning occur and localize the fault.

4.8.2 GLP monitoring

Activating/Deactivating GLP monitoring

Proceed as follows to either activate or deactivate the GLP monitoring for the **temperature**, the **conductivity** and the **gas flow**:

1 Open dialog window

- If several instruments are connected: In the **Control window**, use the menu item **View ▶ Unit x** to select the required instrument.
- Click on the menu item **Tools ▶ GLP test ▶ Properties....**

Tolerance

Indication of the tolerance value for the relevant GLP test. If the result is within the range **Setpoint ± Tolerance**, the test is regarded as passed. If you click on **[Set default]**, the specified standard value is entered in this field.

Additional alert message text

Additional message text which is to be added during the prompt for carrying out the next GLP test.

4.8.3 GLP status

Displaying the GLP status


Proceed as follows to display the status of the GLP monitoring:

1 Open dialog window

- If several instruments are connected: In the **Control window**, use the menu item **View ▶ Unit x** to select the required instrument.
- Click on the menu item **Tools ▶ GLP test ▶ Status....**

The dialog window **GLP status for unit with serial no. x** appears.

Parameter description

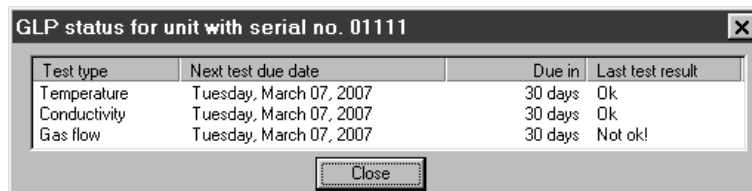

Test type	Next test due date	Due in	Last test result
Temperature	Tuesday, March 07, 2007	30 days	Ok
Conductivity	Tuesday, March 07, 2007	30 days	Ok
Gas flow	Tuesday, March 07, 2007	30 days	Not ok!

Test type

Type of GLP test (**Temperature**, **Conductivity** or **Gas flow**).

Next test due date

Date on which the next GLP test is to be carried out. If the GLP monitoring is not activated, **Disabled** appears in this column.

Due in

Number of days until the next GLP test.

Last test result

Indication whether the test has been passed (**Ok**) or not (**Not Ok!**).



4.8.4 Carrying out GLP tests

4.8.4.1 Temperature

For the **GLP test for temperature measurement** the calibrated temperature sensor and the measuring insert are required (part of the optionally available GLP test set,). For this, the temperature sensor must be connected to the Pt100 connector on the rear of the 743 Rancimat.

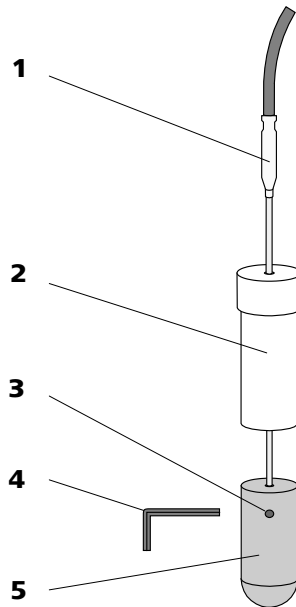


Figure 7 Accessories for GLP test Temperature

1	Pt100 temperature sensor	2	PTFE cylinder
3	Hexagon screw	4	Hexagon key (6.2621.120)
5	Aluminum cylinder		

Preparing the GLP test set

Proceed as follows in order to prepare the GLP test set according to *Figure 7*:

1 Assemble accessories

- Insert the temperature sensor from above into the opening of the PTFE cylinder.
- Place the PTFE cylinder on the aluminum cylinder in such a way that the temperature sensor fits into this opening.
- Push the temperature sensor into the aluminum cylinder as far as the limit stop.

2 Screw on accessories

- Use the hexagon key to lightly tighten the hexagon screw.

Carrying out the GLP test for the temperature measurement


Proceed as follows to carry out the GLP test:



NOTICE

Before starting the GLP test, ensure that the temperature of the inserted GLP test set is stable. If the GLP test set is used in a cold heating block, this condition is fulfilled after the normal heating up time of the heating block and the GLP test set. If the GLP test set, on the other hand, is used in an already heated heating block, it is necessary to wait at least 30 min before starting the GLP test.

1 Select instrument and method

- In the **Control window**, use the menu item **View ▶ Unit x** to select the instrument for which the GLP test is to be carried out.
- Under **Unit x Block A** and **B**, click on the symbol  in order to select the method whose temperature is required for the test.



- If required, adjust the temperature (see "Opening a selected method and adjusting parameters", page 58).

2 Enter calibration points of the temperature sensor

- Click on the menu item **Tools ▶ GLP test ▶ Temperature...** and confirm with **[Next >]**.

The following dialog window appears:

GLP test for unit with serial no. 01111

TEMPERATURE SENSOR DATA
A certified sensor has three points of calibration. Each point consists of a temperature/resistance pair.

Sensor name:

Point 1
T: °C R: Ohm

Point 2
T: °C R: Ohm

Point 3
T: °C R: Ohm

< Back **Next >** Cancel

- Enter a **Sensor name** for the temperature sensor.
- Under **Point 1...3**, enter the **Temperature** and the **Resistance** of the calibration point.
- Confirm the entry with **[Next >]**.

The following dialog window appears:

GLP test for unit with serial no. 01111

TEST PARAMETERS
Select at least one channel per block!

Channels used for test

Block A	Block B
<input type="checkbox"/> Channel 1	<input type="checkbox"/> Channel 1
<input checked="" type="checkbox"/> Channel 2	<input checked="" type="checkbox"/> Channel 2
<input type="checkbox"/> Channel 3	<input type="checkbox"/> Channel 3
<input type="checkbox"/> Channel 4	<input type="checkbox"/> Channel 4


Test duration per channel min

< Back **Next >** Cancel

3 Enter test parameters

- Under **Channels used for test**, select the required channels. One channel per block has to be selected at least.
- Under **Test duration per channel**, enter the required test duration and confirm with **[Next >]**.

The following dialog window appears:

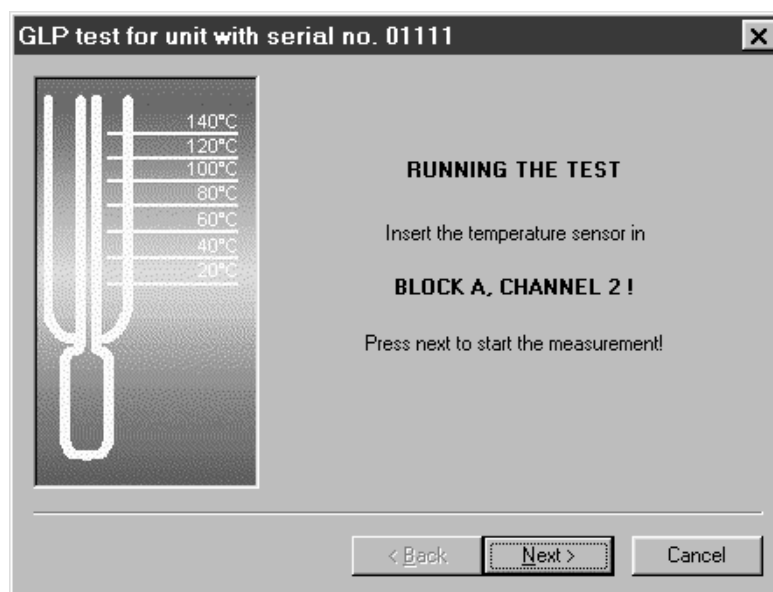


4 Insert GLP test set and start measurement

- Insert the prepared test set (see "Preparing the GLP test set", page 146) in the channel of Block A to be checked.
- Connect the temperature sensor to the Pt100 connector on the rear of the 743 Rancimat.
- In the dialog window **GLP test for unit with serial no. x**, click on **[Next >]**.

The test measurement is started.

As soon as the temperature defined in the method has been reached, the following message appears:

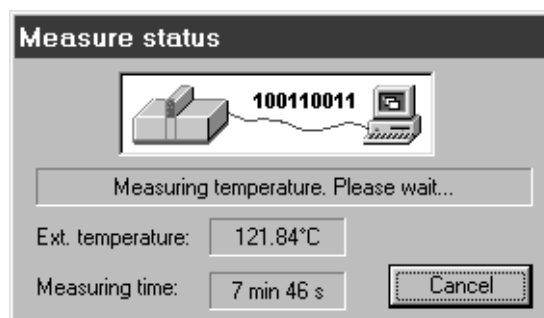

Ext. temperature	The temperature measured with the external temperature sensor.
Measuring time	The time elapsed since the start of the temperature measurement.



5 Carry out measurement for further channels




WARNING

The aluminum cylinder of the GLP test set is very hot. Do not touch!

- As soon as the message appears with the prompt to insert the external temperature sensor together with the measuring insert in the next selected channel, **rapidly carry out the change**.
- Carry out measurement for each of the selected channels.

After the last measurement is completed, the dialog window with the **test results** appears.

6 Confirm or reject results

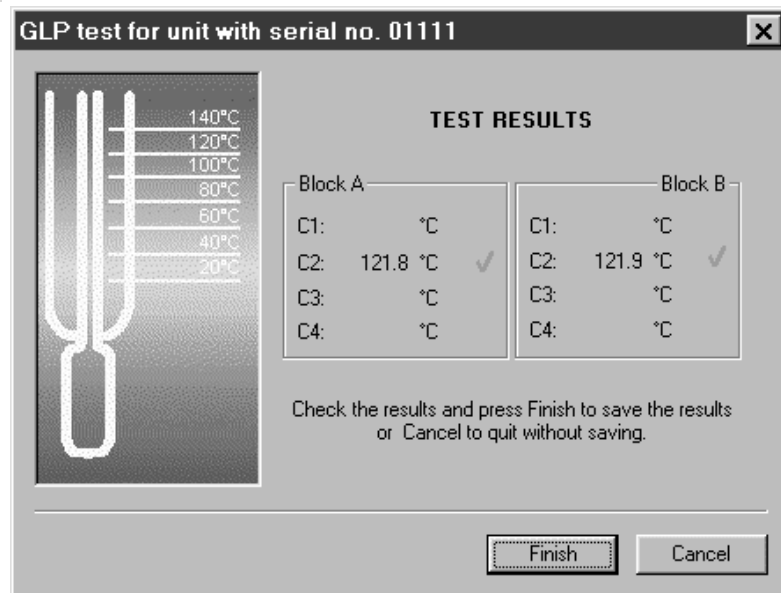

✓	Test passed: The deviation of the measured temperatures is within the specified tolerance.
✗	Test failed: The deviation of the measured temperatures is greater than the specified tolerance.

- Confirm the results with **[Finish]**.

or

- Reject the results with **[Cancel]**.

4.8.4.2 Conductivity

The **GLP test for conductivity measurement** can be carried out either with a **standard solution** with a known conductivity or with the **test resistor 6.2109.030**. The test resistor is part of the optionally available GLP test set. The test resistor must be connected during measurement at the electrode connector (3-2) of the 743 Rancimat.

Carrying out the GLP test for the conductivity measurement

Proceed as follows to carry out the GLP test:



NOTICE

Before carrying out the GLP test **with standard solution** for the first time, the cell constants of the conductivity measuring cells must be determined (*see chapter 4.4.1, page 49*).


1 Select instrument

- In the **Control window**, use the menu item **View ► Unit x** to select the instrument for which the GLP test is to be carried out.
- Carrying out the GLP test with the **test resistor**: continue with step 2.
Carrying out the GLP test with the **standard solution**: continue with step 3.

2 Carry out GLP test with test resistor

- Click on the menu item **Tools ▶ GLP test ▶ Conductivity...** and confirm with **[Next >]**.

The following dialog window appears:

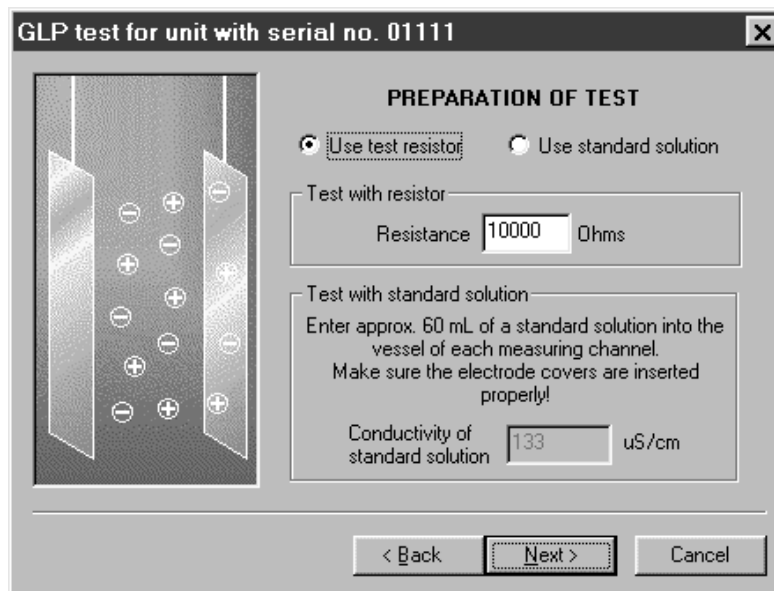

- Select the option **Use test resistor**.
- Under **Resistance**, enter the value of the test resistor in Ohms (10000 Ω for 6.2109.030) and confirm with **[Next >]**.
- Connect the test resistor to the electrode connector (3-2) indicated in the dialog window and confirm with **[Next >]**.
- Continue with step 4.

3 Carry out GLP test with standard solution

- Insert a measuring vessel, each filled with 60 mL standard solution, together with the measuring vessel cover at all measuring position (see chapter 4.6, page 76).

- Click on the menu item **Tools ▶ GLP test ▶ Conductivity...** and confirm with **[Next >]**.

The following dialog window appears:

- Select the option **Use standard solution**.
- Under **Conductivity of standard solution**, enter the conductivity in $\mu\text{S}/\text{cm}$ and confirm with **[Next >]**.

c(KCl) = 1 mmol/L can be used as a standard solution. This is derived from the optionally available conductivity standard 6.2301.060 (KCl 0.1 mol/L) through dilution with distilled water. The conductivity of this diluted solution is:


Temperature	Conductivity
18 °C	127 $\mu\text{S}/\text{cm}$
19 °C	130 $\mu\text{S}/\text{cm}$
20 °C	133 $\mu\text{S}/\text{cm}$
21 °C	136 $\mu\text{S}/\text{cm}$
22 °C	138 $\mu\text{S}/\text{cm}$
23 °C	141 $\mu\text{S}/\text{cm}$
24 °C	144 $\mu\text{S}/\text{cm}$
25 °C	147 $\mu\text{S}/\text{cm}$

The conductivity is measured sequentially at all channels.

After the last measurement is completed, the dialog window with the **test results** appears.



4 Confirm or reject results

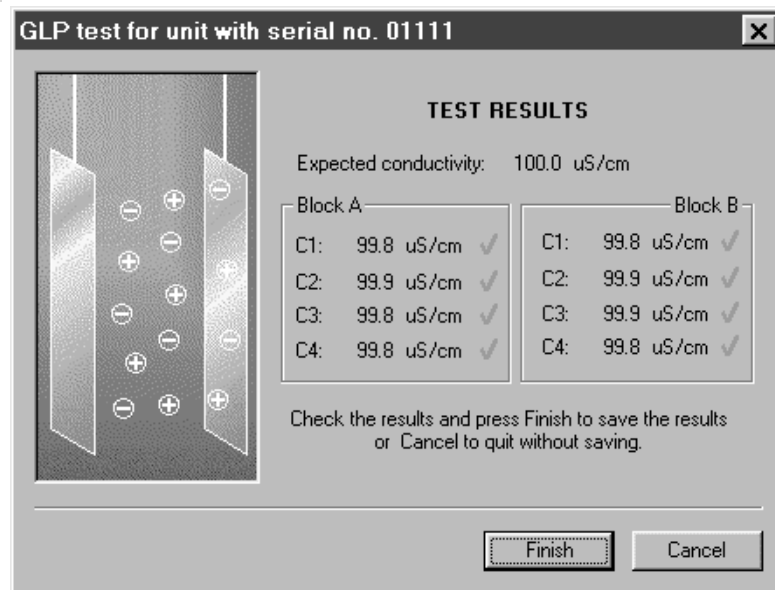

✓	Test passed: The deviation of the measured conductivities is within the specified tolerance.
✗	Test failed: The deviation of the measured conductivities is greater than the specified tolerance.

- Confirm the results with **[Finish]**.

or

- Reject the results with **[Cancel]**.

4.8.4.3 Gas flow

For the **GLP test for gas flow measurement**, you require a gas flow measuring device (not available from Metrohm), which can be used to measure the gas flow at every channel.

Carrying out the GLP test for the gas flow measurement

Proceed as follows to carry out the GLP test:

1 Select instrument and start test

- In the **Control window**, use the menu item **View ► Unit x** to select the instrument for which the GLP test is to be carried out.

- Click on the menu item **Tools ▶ GLP test ▶ Gas flow...** and confirm with **[Next >]**.

The following dialog window appears:

The screenshot shows a dialog window titled "GLP test for unit with serial no. 01111". On the left is a graphic of a gas chromatogram with several peaks of varying heights. The main area is titled "TEST PARAMETERS" and contains a "Gas flow:" label followed by a numeric input field containing "20" and a unit "L/h". At the bottom are three buttons: "< Back", "Next >" (highlighted with a dashed border), and "Cancel".

- Enter the **Gas flow** and confirm with **[Next >]**.

The following dialog window appears:

The screenshot shows the same dialog window, now titled "RUNNING THE TEST". It contains the text: "Please enter the actual flow, measured by your flow meter, in the edit fields below." Below this, there are two columns of input fields labeled "Block A" and "Block B". Each column has four rows labeled "C1:", "C2:", "C3:", and "C4:". Each row has a numeric input field followed by "L/h". In the "Block A" column, the "C1:" field contains "0". In the "Block B" column, all fields contain "0". At the bottom are three buttons: "< Back", "Next >" (highlighted with a dashed border), and "Cancel".


2 Test all channels

- Measure the gas flow sequentially for all channels and enter the values in the corresponding fields K1...K4 in L/h.
- After finishing the measurement, confirm the entries with **[Next >]**.

The dialog window with the **test results** appears.



3 Confirm or reject results

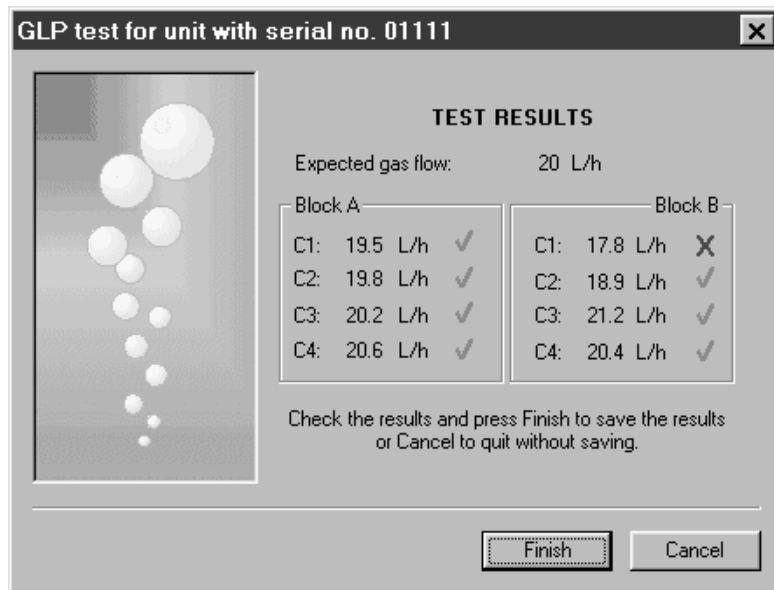

✓	Test passed: The deviation of the measured gas flow values is within the specified tolerance.
✗	Test failed: The deviation of the measured gas flow values is greater than the specified tolerance.

- Confirm the results with **[Finish]**.
- or
- Reject the results with **[Cancel]**.

4.8.5 GLP results

Printing the GLP certificate



NOTICE

To be able to print a test certificate, you have to activate the GLP monitoring (see "Activating/Deactivating GLP monitoring", page 143).

For the selected instrument, you can print a GLP certificate, which contains the following information:

Print date, serial number of the instrument, results of the last GLP tests (with date, test person and test results).

Proceed as follows to print out a test identification:

1 Print GLP certificate

- In the **Control window**, click on the menu item **Tools ▶ GLP test ▶ Print GLP results...**

Displaying the GLP results



NOTICE

If you want an overview of all GLP tests carried out with the connected units, the database **Repos.mrd** must be open. If another database is open, only those GLP tests are displayed which have also been exported into this database during export of the determinations.

Proceed as follows to display the GLP results:

1 Open dialog window with overview

- Open the Results window (see "Opening and closing the Results window", page 29).
- In the **Results window**, click on the menu item **View ▶ GLP** and select the required test results (**Temperature, Conductivity, Gas flow**).

The following dialog windows appear, depending on the selection previously made.

GLP Temperature overview										
Date	Serial number	Channel				Test done / test passed				
		A 1	A 2	A 3	A 4	B 1	B 2	B 3	B 4	
▶ 08.02.2007	01111	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>

GLP Conductivity overview										
Date	Serial number	Channel				Test passed				
		A 1	A 2	A 3	A 4	B 1	B 2	B 3	B 4	
▶ 08.02.2007	01111	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>



GLP Gas flow overview									
Date	Serial number	Channel				Test passed			
		A 1	A 2	A 3	A 4	B 1	B 2	B 3	B 4
▶ 08.02.2007	01111	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>

2 Display detailed results

- Double click on the required GLP test within the fields **Date**, **Serial number** or **Channel**.

The dialog window **GLP Temperature**, **GLP Conductivity** or **GLP Gas flow** appears.

Printing GLP results



NOTICE

To be able to print out the GLP results, you have to activate the GLP monitoring (see "Activating/Deactivating GLP monitoring", page 143).

Proceed as follows to print the GLP results:

1 Open dialog window with overview

- Open the Results window (see "Opening and closing the Results window", page 29).
- In the **Results window**, click on the menu item **View ▶ GLP** and select the required test results (**Temperature**, **Conductivity**, **Gas flow**).

2 Select data

- In the **Results window**, click on the menu item **File ▶ Print....**
If the database contains GLP test results which have been attained with different instruments, the dialog window **Select unit** appears.

- Select the **Serial number** of the required instrument and confirm with **[OK]**.

The following dialog window appears:



- Select the required printing option and confirm with **[OK]**.

Parameter description

Printing options

Selection	Last certificate Certificate of date All temperature GLPs All conductivity GLPs All gas flow GLPs
-----------	--

Last certificate

Printout of the last GLP certificate of the selected overview window. The printout contains the **Serial number** of the instrument, the **Date**, the **Tester** and the **Test result**.

Certificate of date

Printout of the GLP certificate for the entered date. The printout contains the **Serial number** of the instrument, the **Date**, the **Tester** and the **Test result**.

All temperature GLPs

Printout of the detailed results for all GLP tests for temperature measurement.

All conductivity GLPs

Printout of the detailed results for all GLP tests for conductivity measurement.

All gas flow GLPs

Printout of the detailed results for all GLP tests for gas flow measurement.



5 Handling and maintenance

5.1 General information

5.1.1 Care

The 743 Rancimat requires appropriate care. Excess contamination of the instrument may result in functional disruptions and a reduction in the service life of the sturdy mechanics and electronics.

Spillages of chemicals and solvents should be cleaned up immediately. Above all, the plug connections on the rear of the instrument (in particular the mains connection socket) should be protected from contamination.



CAUTION

Although this is extensively prevented by design measures, the mains plug should be unplugged immediately if aggressive media has penetrated the inside of the instrument, so as to avoid serious damage to the instrument electronics. In such cases, the Metrohm Service must be informed.

5.1.2 Maintenance by Metrohm Service

Maintenance of the 743 Rancimat is best carried out as part of an annual service, which is performed by technicians of the Metrohm company. If working frequently with caustic and corrosive chemicals, a shorter maintenance interval could be necessary.

The Metrohm service department offers every form of technical advice for maintenance and service of all Metrohm instruments.

5.2 Replacing the dust filter

The dust filter (3-20) is mounted in the opening marked with **Filter** on the rear of the instrument and serves for filtration of the air sucked in through the air pump. It must be checked at periodic intervals and replaced in the case of more intense contamination (order number: 6.2724.010).

5.3 Regenerating or replacing the molecular sieve



NOTICE

Regenerate the molecular sieve regularly.

The intervals at which you have to regenerate the molecular sieve depends on the **air humidity** in the laboratory and also on the **frequency of use** of the instrument.

The molecular sieve filled in the drying flask (3-11) serves for adsorption of disruptive oxidizing gases as well as of the water from the sucked in air. You can regenerate the molecular sieve in the drying oven at approx. +140...+180 °C for 24 to 48 h. You can order a new molecular sieve under the order number 6.2811.000.



CAUTION

Do **not** fill the hot molecular sieve directly into the drying flask after regeneration, as otherwise the plastic filter on the filter tube will melt.

Wait until the molecular sieve has cooled down before filling.



5.4 Self test when switching on

An internal hardware self test executes after switching on the instrument. Each one of the 7 test steps lasts around one second and is displayed on the instrument number display (2-5) by a combination sample of the 4 display lamps. In the case of an error, the corresponding LEDs flash.

Display	Cause	Remedy
Device 	LED test. If not all LEDs light up during this test, an LED is defective.	Notify Metrohm Service.
Device 	RAM test error.	Switch the instrument off and on again. If the error occurs again, please notify Metrohm Service.
Device 	PROM checksum test error.	Switch the instrument off and on again. If the error occurs again, please notify Metrohm Service.
Device 	BUSY test error.	Switch the instrument off and on again. If the error occurs again, please notify Metrohm Service.
Device 	ADC test error.	Switch the instrument off and on again. If the error occurs again, please notify Metrohm Service.
Device 	EEPROM test error.	Switch the instrument off and on again. If the error occurs again, please notify Metrohm Service.
Device 	Defective mains voltage (deviation > 10 %).	Check power supply.

6 Troubleshooting

6.1 Problems

Problem	Cause	Remedy
The pump is louder than normal.	<i>The air flow is blocked somewhere before or after the pump.</i>	<ul style="list-style-type: none"> Check dust filter (3-20) and, if necessary, replace. Check filter tube (4-4) on the drying flask cover for blockages and, if necessary, free with a gentle tap. Examine FEP tubings (2-6), (3-13), (3-14) and (3-17) for blockages and, if necessary, replace.
	<i>Extra air is sucked in at somewhere else other than the dust filter. There is a leak somewhere in the system before the pump.</i>	<ul style="list-style-type: none"> Check FEP tubings (3-13), (3-14) and (3-17) for cracks, kinks etc. and tighten. If necessary, replace. Place the drying flask cover (3-10) correctly on the drying flask and screw tight.
No air flow can be detected in the reaction vessel (it does not bubble), although the pump is running.	<i>The air supply is blocked.</i>	<ul style="list-style-type: none"> Remove FEP tubing (5-1) from the thread adapter (5-3). A slight air flow must be discerned here. If this is not the case, please contact Metrohm Service. Check FEP tubing (2-6) for blockages. If necessary, clean or replace. Check thread adapter (5-3) and air tube (5-5) on the reaction vessel cover for blockages. If necessary, clean or replace.
	<i>The FEP tubing for the air supply is defective.</i>	Check FEP tubing (2-6) for cracks, kinks etc. If necessary, replace.
	<i>The FEP tubing for the air supply is not connected correctly.</i>	Tighten FEP tubing (2-6) on both sides.
	<i>The air tube (5-5) does not immerse in the sample.</i>	<ul style="list-style-type: none"> Push reaction vessel cover (5-8) down as far as the limit stop. Use more sample.



Problem	Cause	Remedy
No air flow can be detected in the measuring vessel (it does not bubble), although an air flow can be discerned in the reaction vessel.	<i>The connection is blocked.</i>	<ul style="list-style-type: none"> Check tubing connector (5-4) on the reaction vessel cover for blockages and, if necessary, clean. Check silicone tubing (5-2) for blockages and, if necessary, clean. Check tubing adapter (5-11) and PTFE tube (5-17) on the measuring vessel cover for blockages and, if necessary, clean.
	<i>The connection is leaking.</i>	Check silicone tubing (5-2) for leakages and, if necessary, replace.
	<i>The reaction vessel cover (5-8) is not mounted correctly or is too loose.</i>	<ul style="list-style-type: none"> If the reaction vessel cover is oblique or not completely mounted, press down as far as the limit stop. If the reaction vessel cover is loose on the reaction vessel despite correct assembly, the cover has to be replaced.
	<i>The connection is wrongly connected.</i>	<ul style="list-style-type: none"> Ensure that the PTFE tube (5-17) is mounted to the air supply at the opening In (5-13) of the measuring vessel cover. Ensure that the silicone tubing (5-2) is mounted on the tubing adapter, which is mounted in the opening In (5-13). Ensure that the reaction vessel is connected to the measuring vessel belonging to the corresponding measuring place.
The conductivity is displayed in the upper part of the Live window during startup.	<i>The conductivity of the water used is too high.</i>	Check the conductivity of the water used and, if necessary, use deionized water from another source.
	<i>The conductivity measuring cell is contaminated.</i>	Check cell constant of the measuring cell. The cell constant should be between 1.0 and 1.2. If this is not the case, the measuring cell must be cleaned (see chapter 4.6.5, page 84).
The induction times are not reproducible for multiple determinations.	<i>The reaction vessels used are not clean.</i>	<ul style="list-style-type: none"> Free the reaction vessel of particles (dust, cardboard, glass fragments etc.) with compressed air before weighing in the sample. Only use new, unused reaction vessels.



Problem	Cause	Remedy
	<i>The reaction vessels used are scratched on the inside.</i>	Only use new, unused reaction vessels.
	<i>The reaction vessel cover (5-8) is not mounted correctly or is too loose.</i>	<ul style="list-style-type: none"> ▪ If the reaction vessel cover is oblique or not completely mounted, press down as far as the limit stop. ▪ If the reaction vessel cover is loose on the reaction vessel despite correct assembly, the cover has to be replaced.
	<i>The connection to the measuring vessel is not mounted correctly.</i>	Ensure that no air can escape through leaks when transferring from the reaction vessel to the measuring vessel.
	<i>The temperature in different channels of a heating block differs, as there are burn marks at one or more places in the opening of the heating block.</i>	Check temperature in the different positions (see chapter 4.8.4.1, page 146). If necessary, carefully remove the impurities from the cold heating block.
	<i>The temperature in different heating blocks differs.</i>	Determine the temperature correction Delta T for each block separately (see chapter 4.4.2, page 51).
	<i>The sample is not homogeneous.</i>	Homogenize sample.
The stability times are not reproducible for multiple determinations.	<i>The cell constant was not determined or does not correspond to the value entered.</i>	<ul style="list-style-type: none"> ▪ Determine cell constant (see chapter 4.4.1, page 49). ▪ Ensure that the measuring cell is always used in the same channel, so that the cell constant determined once also corresponds to the measuring cell. ▪ Ensure that the measuring cell is not contaminated. If necessary, clean (see chapter 4.6.5, page 84).
	<i>The conductivity measuring cell is contaminated.</i>	Check measuring cell (see chapter 4.8.4.2, page 151) and, if necessary, clean.
	<i>See also: The induction times are not reproducible for multiple determinations.</i>	



Problem	Cause	Remedy
<p>The induction time is longer/shorter than expected.</p>	<p><i>The temperature is not selected correctly.</i></p> <hr/> <p><i>See also: The induction times are not reproducible for multiple determinations.</i></p>	<ul style="list-style-type: none"> ▪ Ensure that the correct method for the determination has been selected. ▪ Check that Temperature and Delta T have been specified correctly in the method (see chapter 4.5.2.1, page 61).
<p>The stability time is longer/shorter than expected.</p>	<p><i>Delta Kappa is not defined correctly.</i></p> <hr/> <p><i>See also: The stability times are not reproducible for multiple determinations.</i></p> <hr/> <p><i>See also: The induction time is longer/shorter than expected.</i></p>	<p>Ensure that the value of Delta Kappa defined in the method is correct (see chapter 4.5.2.2, page 65).</p>
<p>The measurement curves are extremely noisy.</p>	<p><i>The air supply for the measuring solution is directed to the conductivity measuring cell.</i></p> <hr/> <p><i>Gas bubbles adhere to the conductivity measuring cell during measurement.</i></p> <hr/> <p><i>During the measurement, sample evaporates in the reaction vessel and condenses in the measuring vessel. This results in contamination of the conductivity measuring cell, which in turn promotes adherence of gas bubbles.</i></p>	<p>Loosen tubing adapter (5-11) on the measuring vessel cover, turn the PTFE tube (5-17) in such a way that the air is no longer directed to the measuring cell and fix in this position.</p> <hr/> <ul style="list-style-type: none"> ▪ Ensure that the measuring cell is clean and free of fat. If necessary, clean thoroughly (see chapter 4.6.5, page 84). ▪ In some cases ultra pure water contains a large proportion of dissolved air which escapes during measurement. In this case, degas the ultra pure water before the measurement for 5 to 10 min in a vacuum. <hr/> <ul style="list-style-type: none"> ▪ Keep the measuring time as short as possible, by about 4 to 6 h. The induction time can be reduced by about half by increasing the temperature by 10 °C.

Problem	Cause	Remedy
		<ul style="list-style-type: none"> ▪ Reduce the temperature so that less sample evaporates or no sample at all. However, this can substantially extend the measuring time. The induction time approximately doubles by reducing the temperature by 10 °C.
<p>The curve shows a step which means that the induction time is no longer determined correctly.</p>	<p><i>Side reactions occur at the start or during the measurement, which cause the conductivity in the measuring cell to rise.</i></p>	<ul style="list-style-type: none"> ▪ In the method, use the option Evaluation delay or Evaluation suppression (see chapter 4.5.2.2, page 65). ▪ Do not use Endpoint(s) as a stop criterion in the method, but instead a defined Conductivity (e.g. 200 µS/cm) (see chapter 4.5.2.1, page 61). The curves can then also be evaluated manually after finishing the determination.
<p>The curve shows a step at the start of the measurement, which has not occurred in previous measurements.</p>	<p><i>The reaction vessel cover (5-8) and/or the tubing (5-2) still contain residues which are transported into the measuring vessel through the warm air flow when a new measurement is started.</i></p>	<ul style="list-style-type: none"> ▪ Thoroughly clean the reaction vessel cover and the silicone tubing (see chapter 4.6.5, page 84). ▪ Replace the reaction vessel cover and the silicone tubing from time to time.
<p>The induction time is not evaluated automatically, although a significant break point can be noticed in the curve.</p>	<p><i>The option Evaluate induction time is deactivated in the method.</i></p> <p><i>The option Evaluation delay or Evaluation suppression is defined in the method, which prevents the evaluation of the curve in the corresponding time period.</i></p>	<p>Activate the evaluation of the induction time in the method (see chapter 4.5.2.2, page 65).</p> <p>Deactivate the corresponding option in the method (see chapter 4.5.2.2, page 65).</p>
	<p><i>Automatic detection of the induction time is not yet possible.</i></p>	<p>Keep the determination running until the induction time is automatically found.</p>
	<p><i>The curve progression is too flat with the result that automatic detection of the induction time is not possible.</i></p>	<p>Do not use Endpoint(s) as a stop criterion in the method, but instead a defined Conductivity e.g. 200 µS/cm (see chapter 4.5.2.1, page 61). Evaluate the curves afterwards manually.</p>



Problem	Cause	Remedy
		using tangents (see "Setting tangents manually", page 117).
The measurement aborts without an endpoint being found.	<i>The measurement has been stopped manually.</i>	Keep the measurement running until the endpoint is automatically found.
	<i>A time or conductivity is defined as a stop criterion in the method, which was reached before the endpoint.</i>	Deactivate time or conductivity as a stop criterion in the method (see chapter 4.5.2.1, page 61) or increase the corresponding value for the time or conductivity.
	<i>The heating is defective.</i>	Switch the instrument off and on again. If the error occurs again, please contact Metrohm Service.
	<i>The maximum temperature (220 °C) has been exceeded by 10 °C.</i>	Switch the instrument off and on again. If the error occurs again, please contact Metrohm Service.
	<i>Error during self test.</i>	Switch the instrument off and on again. If the error occurs again, please contact Metrohm Service.

7 Technical specifications

7.1 General data

<i>Number of instruments that can be connected</i>	1...4
<i>Number of samples per instrument</i>	1...8 (4 each per heating block)
<i>Sample amount</i>	Several grams / several milliliters

7.2 Temperature regulation and measurement

<i>Range setpoint temperature</i>	50...220 °C
<i>Temperature correction (Delta T)</i>	0...±9.9 °C (can be entered manually or determined automatically using the external temperature sensor)
<i>Temperature measuring range</i>	0...250 °C
<i>Resolution</i>	0.1 °C
<i>Max. deviation of the heating block temperature from the set value (50...220 °C)</i>	±0.3 °C
<i>Reproducibility of the set temperature</i>	typ. < 0.2 °C
<i>Max. temperature difference between different measuring positions per block</i>	typ. < 0.3 °C
<i>Temperature fluctuations</i>	typ. < 0.1 °C (at attained operating temperature, inserted and identically filled reaction vessels and 20 L/h air throughput)



<i>Shutdown temperature</i>	260 ± 11 °C (if this temperature is exceeded, the heating is shut down, and switched on again at 210 ± 11 °C)
<i>Heating up time for the instrument</i>	approx. 45 min (from 20 °C to 120 °C) approx. 60 min (from 20 °C to 220 °C)
<i>Instrument external temperature</i>	< 50 °C (at operating temperature 220 °C)

7.3 Conductivity measurement

<i>Sensor</i>	Conductivity measuring cell, integrated in the measuring vessel cover 6.0913.130
<i>Structure</i>	Conductivity measuring cell with 2 steel electrodes
<i>Measuring principle</i>	AC current measurement with 1 kHz frequency and approx. 1.7 V amplitude (peak to peak)
<i>Cell constant</i>	1.00...1.20 (the exact value can be entered manually or determined automatically)
<i>Measuring range</i>	0...400 µS/cm
<i>Resolution</i>	0.1 µS/cm
<i>Maximum error</i>	±1 % ± 0.5 µS/cm

7.4 Gas flow regulation

<i>Pump</i>	Membrane pump
<i>Adjustable range</i>	7...25 L/h
<i>Max. deviation from the set range</i>	±10 %

7.5 GLP test set

External temperature sensor

<i>Type</i>	Pt100 casing element \varnothing 1.9 mm, in 4-conductor technology; DIN IEC 751 Class B
<i>Calibration accuracy</i>	0...90 °C: \pm 0.02 °C 90...220 °C: \pm 0.03 °C
<i>Max. deviation of the measured temperature from the true value (50...220 °C)</i>	\pm 0.3 °C
<i>Test resistor</i>	10 k Ω

7.6 RS-232 interface

<i>Plug</i>	Sub-D plug, 9-pin (male)
<i>Basic settings</i>	9600 Baud, 8 Bit, 1 stop bit, no parity, XON/XOFF

7.7 Mains connection

<i>Voltage</i>	2.743.0014: 220...240 V \pm 10 % 2.743.0015: 100...120 V \pm 10 %
<i>Frequency</i>	50...60 Hz
<i>Power consumption</i>	450 W
<i>Fuse</i>	Diameter 5 mm, length 20 mm 100...120 V: 2.0 ATH (slow-acting) 220...240 V: 4.0 ATH (slow-acting)



7.8 Ambient temperature

<i>Nominal function range</i>	+5...+45 °C (at 20...80 % humidity)
<i>Storage</i>	-20...+70 °C
<i>Transport</i>	-40...+70 °C

7.9 Housing

<i>Cover material</i>	Polyurethane hard foam (PUR) with flame retardation for fire class UL94VO, CFC-free
<i>Base material</i>	Steel, painted
<i>Width</i>	405 mm
<i>Height</i>	268 mm (without accessories) 353 mm (with accessories)
<i>Depth</i>	466 mm
<i>Weight</i>	20.2 kg (without accessories) 27.6 kg (with accessories)

8 Accessories

Up-to-date information on the scope of delivery and optional accessories for your product can be found on the Internet. You can download this information using the article number as follows:

Downloading the accessories list

- 1 Enter <https://www.metrohm.com/> into your Internet browser.
- 2 Enter the article number (e.g. **743**) into the search field.
The search result is displayed.
- 3 Click on the product.
Detailed information regarding the product is shown on various tabs.
- 4 On the **Included parts** tab, click on **Download the PDF**.
The PDF file with the accessories data is created.



NOTICE

Once you have received your new product, we recommend downloading the accessories list from the Internet, printing it out and keeping it together with the manual for reference purposes.

- Login
 For the first time 22
- M**
-
- Measuring vessel
 Equip 13
- Method 26
 Create 56
 Delete 60
 Open 58
 Rename 58
 Save 57
- Method data
 Display 104
 Export 134
 Print 130
- Method parameters
 Adjust 57, 61
 Adjust during the determination 85
 Print 61
- Molecular sieve
 Regenerate 12, 161
- Mouse functions 32
- Multiple graph
 Display 113
 Print 131
- O**
-
- Oil
 Pure, clear oils 77
- P**
-
- Parameter description
 Determination overview 96
 Method 61
- Parameters
 Adjust 57, 61
 Adjust during the determination 85
 Print 61
- Password
 Set 22
- PC
 Connect 20
- Power connection 19
- Print 129
 Extrapolation results 133
 GLP certificate 156
- GLP results 158
 Instrument information 43
 Method parameters 61
- Program
 Optimize 42
- Program number 44
- Program start 25
 For the first time 22
- Protocol 32
- R**
-
- Reaction vessel
 Equip 13
- Recalculation 26, 122
- Reevaluation 26, 117
- Report
 Print instrument information 44
 Print method information ... 72
- Results 26
- Results window 28
 Close 29
 Menus 30
 Open 29
 Structure 29
 Symbols 30
- Rights
 Activate/Deactivate 37
- S**
-
- Safety instructions 4
- Sample identification
 Clear list 83
 Enter 83
- Samples, prepare 77
 Emulsion fats 80
 Non-liquid, pure fats 77
 Pure oil 77
 Samples containing oils and fats 78
- Self test 162
- Sensor calibration data 54
- Serial number 44
- Service 5
- Service diagnosis 43
- Shutdown temperature 170
- Single graph
 Display 113
- Print 131
- Software
 Installation 20
 Start 25
- Stability time 66
 Live graph 115
 Multiple graph 114
 Recalculate 123
 Single graph 114
- Standard time
 Recalculate 124
- Standart time 71
- Start delay
 Method 63
- Start mode
 Method 63
- Start options
 Method 63
- Status overview 45
- Stop criteria
 Method 64
- Supply voltage 6
- Switch off 19
- Switch on 19
- System requirements 20
- T**
-
- Temperature
 Method 62
 Record 41
- Temperature correction
 Determine 51
- Temperature measuring
 Measuring range 169
 Reproducibility 169
 Resolution 169
- Timer 38
- U**
-
- User
 Add 37
 Delete 38
- User group
 Add 36
 Adjust access rights 36
 Delete 38
- Z**
-
- Zooming 32