



Application Note AN-RS-033

Raman and SERS identification of YABA, a popular street drug

Two chemical analyses from one tablet

Yaba, which means «crazy medicine» in Thai, is a small, colorful tablet containing a potent mixture of caffeine and methamphetamine. It is produced in Southeast Asia, where it is a popular drug of abuse and is actively targeted by police squads. Two strong and highly addictive stimulants make up Yaba: caffeine, which comprises up to 60% of each tablet, and methamphetamine at approximately 20%. Identification of two active ingredients in different proportions in a tablet, complicated by excipients and colored coatings, could be an analytical nightmare.

With handheld Raman, bulk material identification is achieved in seconds onsite with simple point-and-shoot analysis. SERS (surface-enhanced Raman spectroscopy) analysis is used to detect the minor component in mixtures without interference from fillers, dyes, and coatings. **MIRA DS is uniquely capable of both analyses**— Raman testing positively identifies caffeine in Yaba, while methamphetamine can be detected with SERS sampling. This application describes quick, dual analysis of Yaba tablets with MIRA DS.

Handheld Raman is the perfect tool for instant, onsite analysis of street drugs. MIRA DS can easily penetrate the colored coating of tablets to analyze the interior. Raman systems will effectively identify the dominant

component(s) in a mixture. With ID Kit and the SERS Attachment for MIRA DS, minor or trace components of a mixture can be revealed.

SAMPLING WITH RAMAN

For Raman analysis of Yaba, the tablet was sampled directly by laying it on a horizontal surface, positioning the Right Angle attachment over it, and collecting data. Smart Acquire on MIRA DS simplifies material identification: arm the laser, press acquire, and the system automatically determines optimal acquisition parameters for best quality spectra. Then, the instrument processes the data, performs library searches, and publishes a result with associated color-coded warnings—all in less than a minute.

The initial test of Yaba with Raman yielded a positive identification of caffeine, with a high Hit Quality Index (HQI) = 0.81, meaning that sample and library spectra were well correlated (Figure 1).

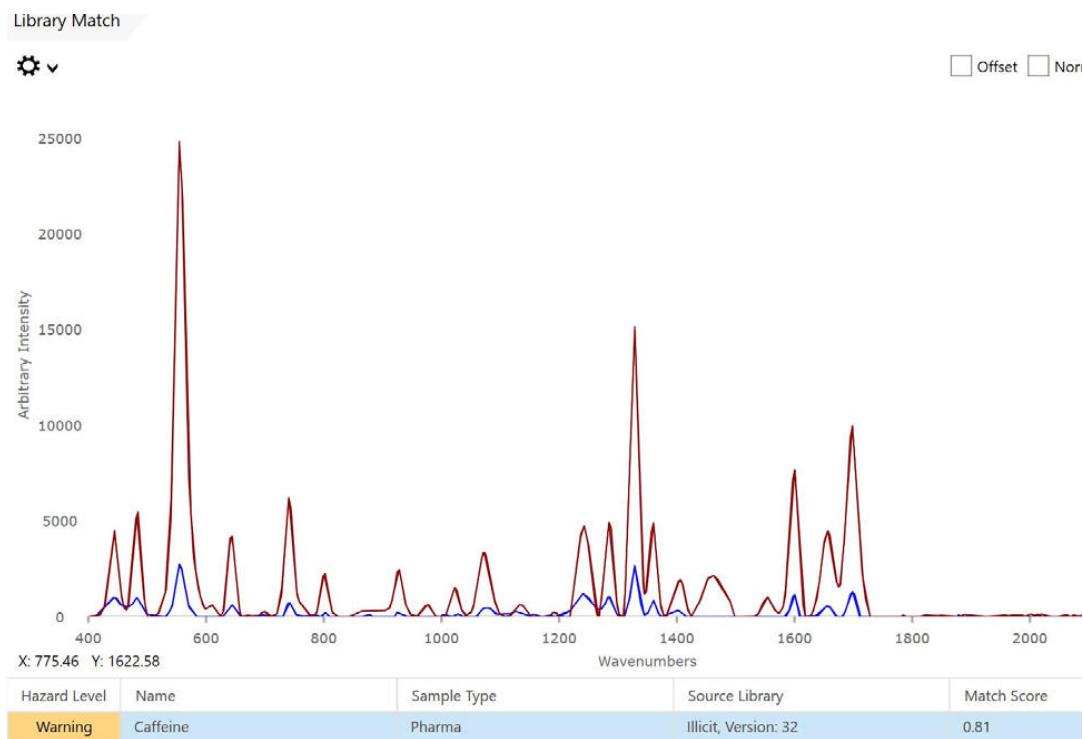


Figure 1. Yaba sample (blue) matched to caffeine (red) in the Illicit Library in Mira Cal DS.



Figure 2. Actual screenshot of identification of caffeine in Yaba with MIRA DS. Caffeine is a chemical commonly associated with illicit drugs. The yellow warning background provides immediate, actionable information about the nature of the sample.

SAMPLING WITH SERS

SERS typically requires that materials be solvated for adsorption to SERS substrates, therefore all materials necessary for this application are included in ID Kit for MIRA DS. ID Kit is used with the SERS Attachment, which automatically activates the SERS Operating Procedure when connected to MIRA DS.

Sampling was straightforward: part of a Yaba tablet was crushed and dissolved in ethyl acetate, then this solution was applied to a silver P-SERS strip. The P-SERS strip was inserted into the SERS attachment on MIRA DS for data collection. With SERS analysis, it was possible to obtain a positive identification of methamphetamine, the minor active component in the Yaba tablet.



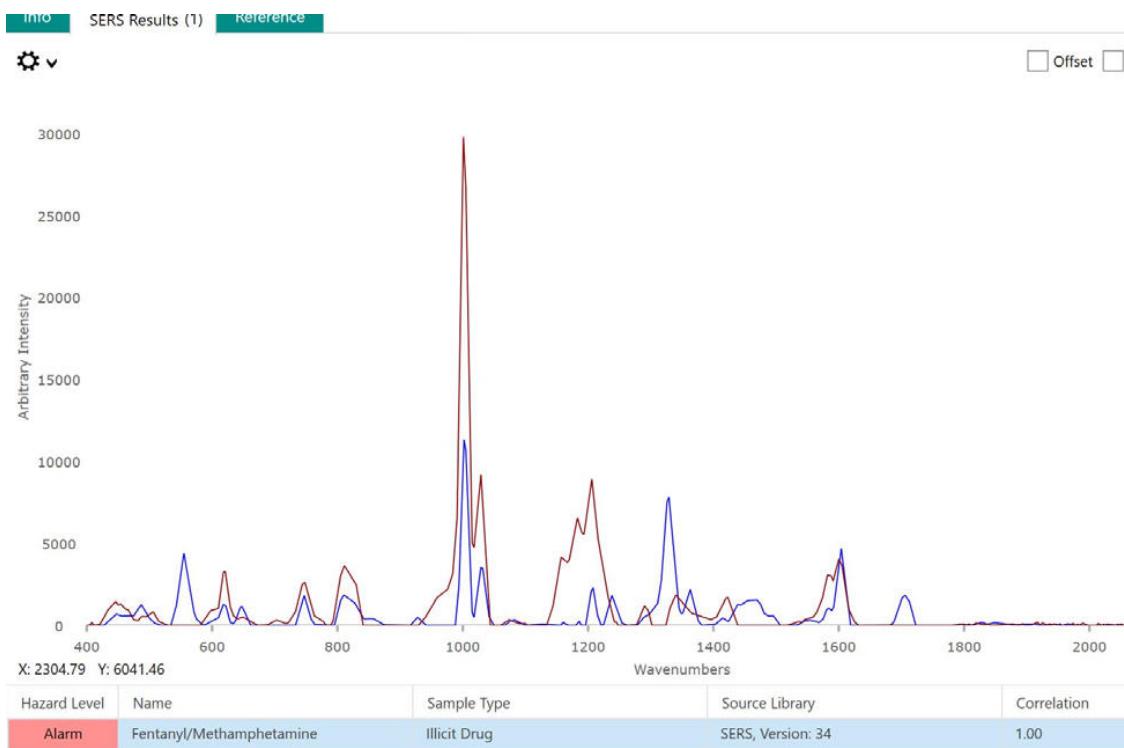


Figure 3. Identification of methamphetamine (sample in blue, library spectrum in red) in Yaba with SERS.

CONCLUSION

Handheld Raman can play an important role in field testing for addictive and potentially dangerous street drugs. MIRA DS helps to establish presumptive evidence of narcotics, which is then established through further testing.

Not only can MIRA DS quickly and accurately identify components in a suspicious tablet, it can be used for through-container testing. This helps to protect defense and security professionals from unknown illicit or otherwise dangerous substances in the field.

MIRA DS also excels at white powder analysis. Fentanyl is cut with heroin, which is then cut with baking soda (sodium bicarbonate), sugar, caffeine, and starches. When a well-known cutting agent is detected during white powder analysis with handheld Raman, SERS can subsequently identify the active opioid(s). This is an excellent illustration of two important functions of the MIRA DS handheld Raman system. One compact instrument can be used—even by non-technicians in the field—to quickly and easily perform both bulk Raman identification and SERS trace analysis with great accuracy.



CONTACT

Metrohm Nordic ApS
Lyskær 3C. 1. th.
2730 Herlev

mail@metrohm.dk

CONFIGURATION



MIRA DS Advanced

The Metrohm Instant Raman Analyzer (MIRA) DS is a ruggedized, high-performance, handheld Raman spectrometer used for rapid, nondestructive determination of illicit materials, e.g. drugs, explosives, starting materials, and hazardous agents. Despite the small size of the instrument, MIRA DS is extremely rugged and features a high-efficiency spectrograph equipped with our unique Orbital-Raster-Scan (ORS) technology.

The Advanced package includes a calibration standard, universal attachment for analyses in bottles or bags or for direct analysis, and the right-angle attachment, ideal for running samples on a surface and/or in a bag. Class 3B operation. MIRA DS supports Metrohm handheld Raman libraries.



ID Kit – Ag P-SERS

The ID Kit - Ag P-SERS contains the components a Mira / Misa user requires to perform a SERS analysis using silver P-SERS strips. The kit contains a disposable spatula, dropper, sample vials and 2 silver P-SERS strips.