



Application Note AN-V-229

# Antimony(III) in drinking water

## Straightforward determination in the low ng/L range on the scTRACE Gold

The toxicity of antimony depends on its oxidation state: antimony(III) is more toxic than antimony(V). Due to its carcinogenicity, EU legislation specifies 5 µg/L and the World Health Organization (WHO) sets a maximum concentration of 20 µg/L as the Sb(III) limit value in drinking water.

Straightforward determination using anodic stripping voltammetry provides a fast (analysis time under 10 minutes) and an ultra-sensitive tool for monitoring the antimony(III) concentration in drinking water. Already with a 30 s deposition time, the limit of detection is

around 0.1 µg/L and can be lowered even further. The linear range ends at ca. 20 µg/L. This determination is performed on the scTRACE Gold: a combined sensor containing working, reference, and auxiliary electrodes integrated on a single ceramic substrate. The scTRACE Gold electrode does not need extensive maintenance such as mechanical polishing. Measurements can be performed in the laboratory with the 884 Professional VA, or alternatively in the field with the 946 Portable VA Analyzer. This method is suited for manual or automated systems.

## SAMPLE

Drinking water, mineral water, seawater

## EXPERIMENTAL

The water sample and the supporting electrolyte are pipetted into the measuring vessel. The determination of antimony(III) is carried out with the 884 Professional VA or with the 946 Portable VA Analyzer using the parameters specified in **Table 1**. The concentration is determined by two additions of an antimony(III) standard addition solution. The scTRACE Gold is electrochemically activated prior to the first determination.



**Figure 1.** 946 Portable VA Analyzer



**Figure 2.** 884 Professional VA, fully automated for VA analysis

**Table 1.** Parameters

Parameter	Setting
Mode	DP – Differential Pulse
Deposition potential	-0.1 V
Deposition time	30 s
Start potential	-0.1 V
End potential	0.2 V
Peak potential Sb(III)	0.06 V


## ELECTRODES

- scTRACE Gold

## RESULTS

At a 30 s deposition time, this method is suitable for the determination of antimony(III) in water samples in

concentrations from  $\beta(\text{Sb(III)}) = 0.1\text{--}10 \mu\text{g/L}$ .

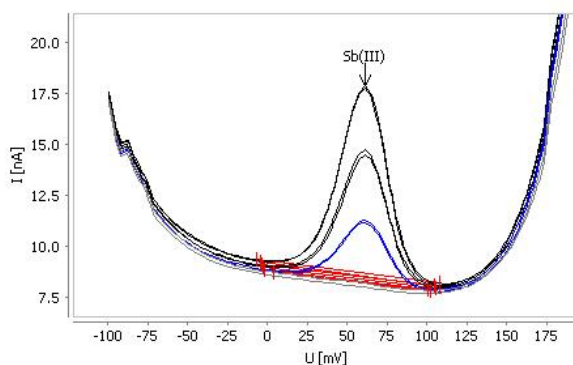

**Figure 3.** Determination of antimony(III) in tap water spiked with 1  $\mu\text{g/L}$  (30 s deposition time)

**Table 2.** Result

Sample	Sb(III) ( $\mu\text{g/L}$ )
Tap water spiked with 1 $\mu\text{g/L}$ Sb(III)	0.94

## CONTACT

Metrohm Deutschland  
In den Birken 3  
70794 Filderstadt

[info@metrohm.de](mailto:info@metrohm.de)

## CONFIGURATION



### 884 Professional VA manual für Multi-Mode-Elektrode (MME)

884 Professional VA manual für Multi-Mode-Elektrode (MME) ist das Einstiegsgerät in die High-End-Spurenanalytik mit Voltammetrie und Polarographie mit der Multi-Mode-Elektrode pro, der scTRACE Gold oder der Bismut-Tropfenelektrode. Die bewährte Metrohm-Elektrodenteknik in Kombination mit einem leistungsfähigen Potentiostaten/Galvanostaten und der extrem flexiblen viva-Software eröffnet neue Perspektiven für die Bestimmung von Schwermetallen. Der Potentiostat mit zertifiziertem Kalibrator justiert sich vor jeder Messung automatisch neu und garantiert höchstmögliche Präzision.

Mit dem Gerät können auch Bestimmungen mit rotierenden Scheibenelektroden durchgeführt werden, zum Beispiel Bestimmungen von organischen Additiven in galvanischen Bädern mit «Cyclic Voltammetric Stripping» (CVS), «Cyclic Pulse Voltammetric Stripping» (CPVS) und Chronopotentiometrie (CP). Der austauschbare Messkopf ermöglicht den schnellen Wechsel zwischen den verschiedenen Applikationen mit unterschiedlichen Elektroden.

Zur Steuerung, Datenerfassung und -auswertung wird die Software **viva** benötigt.

Das 884 Professional VA manual für MME wird mit umfangreichem Zubehör und Messkopf für die Multi-Mode-Elektrode pro geliefert. Elektrodensatz und **viva**-Lizenz sind separat zu bestellen.



### VA-Elektrodenausrüstung mit scTRACE Gold für Professional-VA-Geräte

Kompletter Elektrodensatz für die Bestimmung von Arsen oder Quecksilber. Enthält Halter für scTRACE Gold, scTRACE Gold, Rührer und Messgefäß.



### 946 Portable VA Analyzer (scTRACE Gold)

Tragbarer Metallanalysator für die Bestimmung von Schwermetallen wie Arsen, Quecksilber, Kupfer, Blei, Zink, Nickel, Kobalt, Eisen, Bismut oder Antimon im Spurenbereich. Geräteversion für die scTRACE Gold. Das System besteht aus Potentiostat und separatem Messstand mit eingebautem Rührer und austauschbarer Elektrode. Das Gerät wird mit der Portable VA Analyzer Software betrieben. Die Stromversorgung erfolgt über den USB-Anschluss und über die eingebaute wiederaufladbare Batterie. Das Gerät wird mit allem notwendigen Zubehör in einem Tragekoffer ausgeliefert.