



Application Note AN-RS-029

# Trace Detection of Malathion on Corn

## Protecting consumer safety with Misa

Malathion is an insecticide widely used on a broad spectrum of plant species. Although classified as having low toxicity, ingestion or acute skin exposure can be dangerous to humans. Several studies have implicated chronic exposure to malathion in the development of certain cancers. Maximum residue limits for malathion have been enacted by the regulatory agencies of several countries: the US Food and Drug Administration sets maximum residue limits at 8 µg/g in foods, while the EU has a considerably

more stringent limit of 20 ng/g.

SERS is an accepted method for detection of malathion on fruit and vegetable surfaces. Misa (Metrohm Instant SERS Analyzer), which requires minimal laboratory chemicals and consumables and provides an extremely user-friendly interface, is an excellent SERS solution for trace detection of food adulterants. Misa is a formidable advancement in cost and convenience related to food safety testing and data analysis.

## INTRODUCTION


This application note describes a simulated test procedure for detecting malathion sprayed on corn kernels. The assay is based on the acquisition of SERS-

specific spectra for malathion in acetone extracts using Misa and gold nanoparticles (Au NPs).

## REFERENCE SPECTRUM AND LIBRARY CREATION

To establish a reference spectrum, a pure malathion standard at 100 µg/mL in ethanol was analyzed using

Au NPs. The unique SERS spectrum shown in **Figure 1** can be used to create a library entry for malathion.

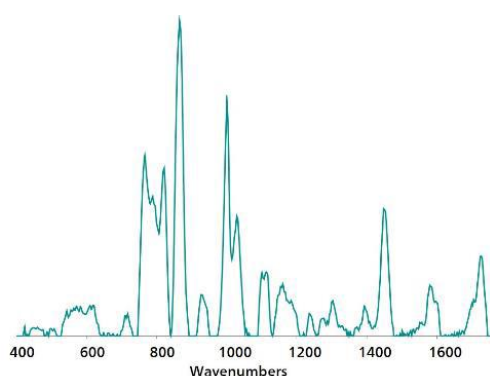

**Figure 1.** Standard Au NP SERS reference spectrum of malathion.

## EXPERIMENT

A stock solution of malathion in acetone was sprayed onto field corn kernels to yield a range of test samples from 1–20 µg/g (concentrations calculated with respect to mass of corn kernels). 0.25 mL of acetone was added to samples in capped glass vials, which were swirled occasionally over a period of 10 minutes to facilitate extraction. At the end of this time, 100 µL of the acetone extract was transferred to a second glass vial and dried on a hot plate. The residue was resuspended in 450 µL of Au NPs and 50 µL of 0.5 mol/L NaCl, the vial was gently shaken to mix, and then immediately placed into the vial attachment on Misa for measurement.




**Table 1.** Experimental parameters

Instrument		Acquisition	
Firmware	0.9.33	Laser Power	5
Software	Misa Cal V1.0.15	Int. Time	10 s
Misa Vial Attachment	6.07505.040	Averages	10
ID Kit - Au NP	6.07506.440	Raster	ON

## RESULTS

Overlaid baseline-corrected spectra acquired for malathion recovered from corn kernels reveal high-resolution malathion detection down to 5 µg/g (Figure 2). Note at these low concentrations, SERS

spectra are very sensitive to any other SERS-active moieties present, including organic materials dissolved with the target compound and the SERS substrate itself.

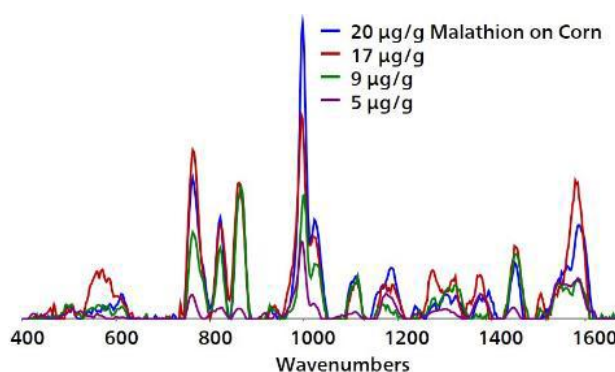

**Figure 2.** Overlaid baseline-corrected spectra acquired from Au NPs show detection of malathion on field corn kernels to 5 µg/g.

## FIELD TEST PROTOCOL

### Detection of malathion in the field

Place 2–3 pieces of corn in a vial and fill the vial halfway full with acetone, and allow to rest for 5 to 10 minutes, swirling occasionally. With a pipette, remove half of the solvent to a *clean, dry vial* and evaporate to

dryness on a hotplate. Fill this vial halfway full with Au NPs and add 2 drops of NaCl solution, then cap and shake the vial gently to mix. Insert into the vial attachment on Misa for measurement.

**Table 2.** Requirements for field test protocol

ID Kit - Au NP	6.07506.440
includes:	Gold nanoparticles (Au NP)
	Scoop
	Disposable pipettes
	2 mL glass vials
Reagents	
Acetone	
NaCl solution	3 g NaCl in 100 mL water
Test settings	Use ID Kit OP on MISA

## CONCLUSION

Misa offers a facile, green, and economical method for sensitive detection of malathion sprayed on corn ears. Based on the unoptimized protocol reported in this application note, Misa provides sufficient sensitivity

for detecting malathion at concentrations that approximate or exceed the US maximum residue limit for sweet corn.

## CONTACT

Metrohm Deutschland  
In den Birken 3  
70794 Filderstadt

[info@metrohm.de](mailto:info@metrohm.de)

## CONFIGURATION



### MISA Advanced

Metrohm Instant SERS Analyzer (MISA) ist ein hochleistungsfähiges, tragbares Analysensystem zur schnellen Detektion / Identifizierung von illegalen Substanzen, Lebensmittelzusatzstoffen und Lebensmittelverunreinigungen im Spurenbereich. MISA verfügt über einen hocheffizienten Spektrographen, der mit der einzigartigen Orbital-Raster-Scan (ORS)-Technologie von Metrohm ausgestattet ist. Er hat einen minimalen Platzbedarf und eine verlängerte Batterielebensdauer, perfekt für Tests vor Ort oder mobile Laboranwendungen. MISA bietet verschiedene Laser-Klasse-1-Aufsätze für flexible Probenahmeoptionen. Der Betrieb des Analysators ist über BlueTooth oder USB-Konnektivität möglich.

Das MISA Advanced-Paket ist ein Komplettpaket, das es dem Anwender ermöglicht, SERS-Analysen mit Metrohms Nanopartikelösungen und P-SERS-Streifen durchzuführen.

Das MISA Advanced-Paket enthält einen MISA Vial-Aufsatz, einen P-SERS-Aufsatz, einen ASTM-Kalibrierstandard, ein USB-Minikabel, ein USB-Netzteil und die MISA Cal-Software zum Betrieb des MISA-Geräts. Ein robuster Schutzkoffer zur sicheren Aufbewahrung des Instruments und des Zubehörs wird ebenfalls mitgeliefert.



### ID Kit – Au NP

Das ID Kit - Au NP enthält die Komponenten, die ein Mira/Misa-Benutzer benötigt, um eine SERS-Analyse mit kolloidaler Goldlösung durchzuführen. Der Kit enthält einen Einwegspatel, eine Tropfpipette, Probenfläschchen und eine Flasche mit Gold-Kolloid