



Application Note AN-NIR-113

Research octane number (RON) determination in isomerate

NIRS offers users fast, efficient analysis with low running costs

Light naphtha isomerization is used by refineries to produce high-octane isomerate products which meet current gasoline specifications. Isomerization increases the octane value of light naphtha by increasing the degree of branching of paraffin molecules. The research octane number (RON) of the target product is dependent on various plant production parameters (e.g., temperature or hydrogen to hydrocarbon ratio). To optimize the plant

process, a reliable and quick analytical method is key. The standard method to determine RON in isomerate is with expensive and maintenance-intensive engines. In contrast to this, the research octane number can also be analyzed by near-infrared spectroscopy (NIRS). NIRS provides accurate results within one minute without the need for any sample preparation or chemicals.

EXPERIMENTAL EQUIPMENT

63 different isomerate samples with varying RON values were measured with the Metrohm DS2500 Liquid Analyzer (Figure 1) in transmission mode over the full wavelength range of 400–2500 nm. The built-in temperature controller ensured measurement stability with a constant sample temperature of 35 °C.

For convenience, disposable vials with a pathlength of 8 mm were used which made a cleaning procedure obsolete. The Vision Air Complete software package from Metrohm was used for data acquisition and prediction model development.

Table 1. Hardware and software equipment overview.

| Equipment | Article number |
|--------------------------|----------------|
| DS2500 Liquid Analyzer | 2.929.0010 |
| DS2500 Holder 8 mm vials | 6.7492.020 |
| Vision Air 2.0 Complete | 6.6072.208 |



Figure 1. Metrohm DS2500 Liquid Analyzer used for the determination of research octane number (RON) in isomerate samples.

RESULT

The obtained Vis-NIR spectra (Figure 2) were used to create a prediction model for the quantification of research octane number in isomerate. The quality of the prediction models was evaluated using correlation diagrams based on the cross-validation

algorithm. A value of $R^2 > 0.98$ displays a high correlation between the Vis-NIR prediction and the reference ASTM method. The respective figures of merit (FOM) display the expected precision during routine analysis (Figure 3).

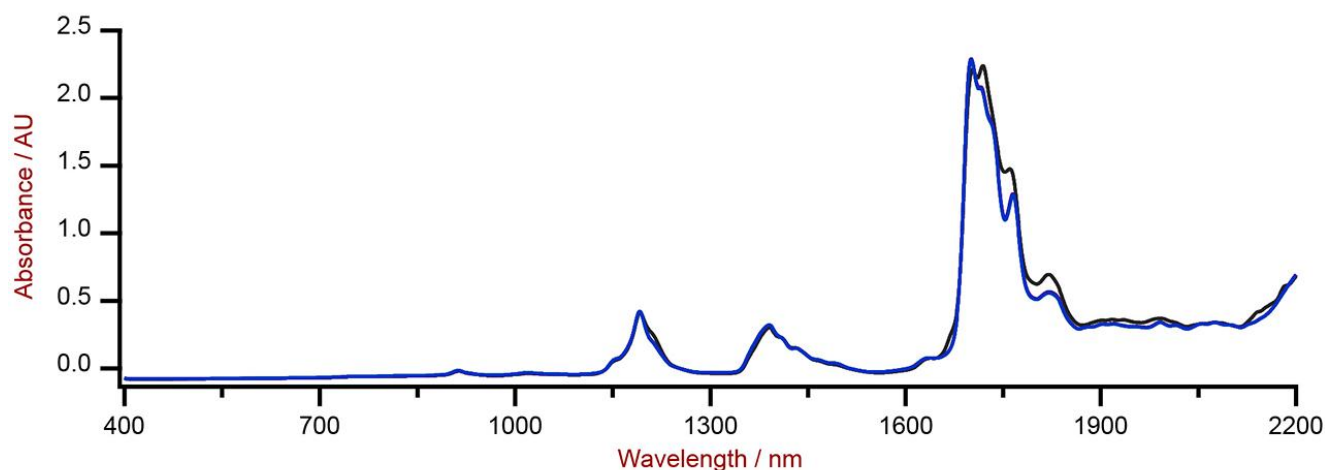


Figure 2. Selection of Vis-NIR spectra of isomerate samples analyzed on a DS2500 Liquid Analyzer with 8 mm vials.

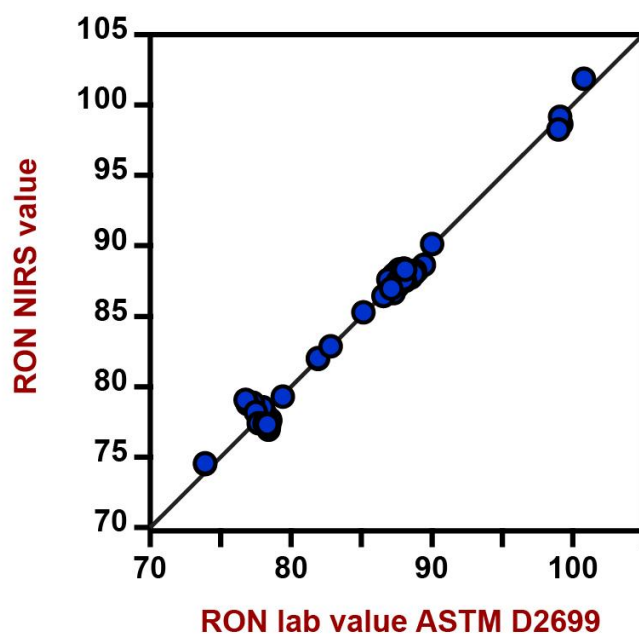


Figure 3. Correlation diagram and the respective figures of merit for the prediction of RON value using a DS2500 Liquid Analyzer. The lab value was evaluated according to ASTM D2699.

| Figures of Merit | Value |
|------------------------------------|-------|
| R^2 | 0.986 |
| Standard Error of Calibration | 0.73 |
| Standard Error of Cross-Validation | 0.76 |

CONCLUSION

This Application Note demonstrates the feasibility of NIR spectroscopy for the analysis of RON in isomate samples. In comparison to the conventional method, the time to result (Table 2) is a major advantage of

Vis-NIR spectroscopy. With NIRS, a single measurement is performed within one minute, while the CFR engine test is much longer.

Table 2. Time to result for the determination of RON value with the standard reference method ASTM D2699.

| Parameter | Method | Time to result |
|-----------|-----------------|-----------------------|
| RON | CFR engine test | 30 minutes per sample |

CONTACT

Metrohm AG
Ionenstrasse
9100 Herisau

info@metrohm.com

CONFIGURATION



DS2500 Liquid Analyzer

Robust near-infrared spectroscopy for quality control, not only in laboratories but also in production environments.

The DS2500 Liquid Analyzer is the tried and tested, flexible solution for routine analysis of liquids along the entire production chain. Its robust design makes the DS2500 Liquid Analyzer resistant to dust, moisture and vibrations, which means that it is eminently suited for use in harsh production environments.

The DS2500 Liquid Analyzer covers the full spectral range from 400 to 2500 nm, heats samples up to 80°C and is compatible with various disposable vials and quartz cuvettes. The DS2500 Liquid Analyzer is thus adaptable to your individual sample requirements and helps you obtain accurate and reproducible results in less than one minute. The integrated sample holder detection and the self-explanatory Vision Air Software also ensure simple and safe operation by the user.

In the case of larger-sized sample quantities, productivity can be considerably increased by using a flow-through cell in combination with a Metrohm sample robot.



DS2500 Holder 8 mm vials

Intelligent holder for disposable glass vials with 8 mm diameter



Vision Air 2.0 Complete

Vision Air - Universal spectroscopy software.

Vision Air Complete is a modern and simple-to-operate software solution for use in a regulated environment.

Overview of the advantages of Vision Air:

- Individual software applications with adapted user interfaces ensure intuitive and simple operation
- Simple creation and maintenance of operating procedures
- SQL database for secure and simple data management

The Vision Air Complete version (66072208) includes all applications for quality assurance using Vis-NIR spectroscopy:

- Application for instrument and data management
- Application for method development
- Application for routine analysis

Additional Vision Air Complete solutions:

- 66072207 (Vision Air Network Complete)
- 66072209 (Vision Air Pharma Complete)
- 66072210 (Vision Air Pharma Network Complete)