



Application Note AN-NIR-088

# Quality Control of CBD oils

## Fast and easy determination of cannabinoid content

Cannabidiol (CBD) is a popular natural remedy used in many pharmaceutical, food, and cosmetic products. CBD is just one of over 100 chemical compounds found in the cannabis plant. Unlike tetrahydrocannabinol (THC), CBD is not psychoactive. This characteristic makes CBD an appealing option for those who are looking for relief from pain and other symptoms without the mind-altering effects associated with consuming marijuana or resin

concentrates. CBD oil is made by extracting the compound from the plant, then diluting it with a carrier oil (e.g., coconut or hemp seed oil).

The standard HPLC method requires 45 minutes to perform by highly trained analysts. In contrast to the primary method, Vis-NIR spectroscopy is a cost-efficient and fast analytical solution for the determination of cannabinoid content in oils.

## EXPERIMENTAL EQUIPMENT

17 samples of three different CBD carrier oils (hemp, fish, and MCT (medium-chain triglycerides) oil) were measured in transmission mode with a DS2500 Liquid Analyzer. The built-in temperature control was set to 40 °C to acquire reproducible spectra. For convenience, disposable vials with a path length of 8 mm were used, which made cleaning of the sample vessels unnecessary. The Metrohm software package Vision Air Complete was used for all data acquisition and prediction model development.



**Figure 1.** DS2500 Liquid Analyzer and a sample filled in a disposable vial.


**Table 1.** Hardware and software equipment overview

Equipment	Metrohm number
DS2500 Liquid Analyzer	2.929.0010
DS2500 Holder 8 mm vials	6.7492.020
Disposable vials, 8 mm	6.7402.000
Vision Air 2.0 Complete	6.6072.208


## RESULTS

All 17 measured Vis-NIR spectra (**Figure 2**) were used to create a prediction model for quantification of the cannabinoid content. The quality of the prediction models was evaluated using cross-validation, which

display a very high correlation between Vis-NIR prediction and primary method values. The respective figures of merit (FOM) display the expected performance of a prediction during routine analysis.

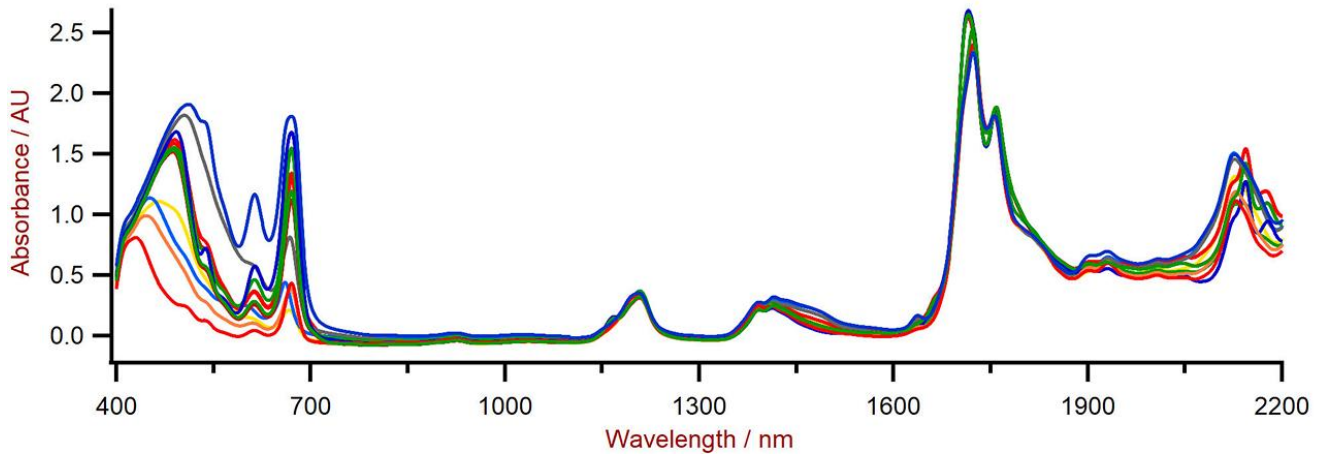

**Figure 2.** Vis-NIR spectra of CBD oils with varying cannabinoid content measured on a DS2500 Liquid Analyzer.

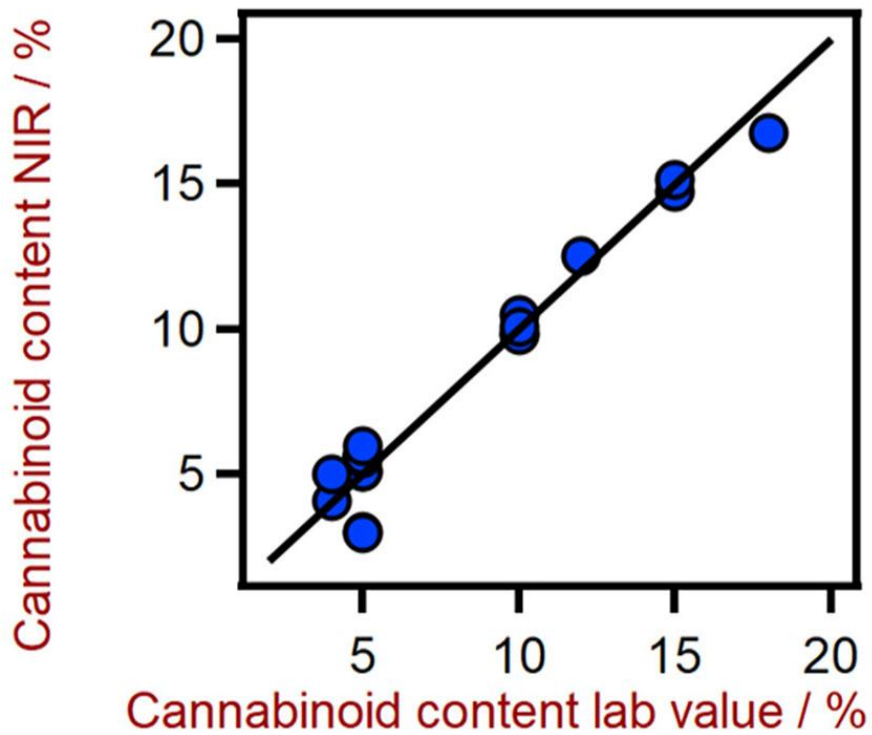

**Figure 3.** Correlation diagram for the prediction of cannabinoid content in CBD oils using a DS2500 Liquid Analyzer.

**Table 2.** Figures of merit for the prediction of cannabinoid content in CBD oils using a DS2500 Liquid Analyzer.

Figures of Merit	Value
R <sup>2</sup>	0.959
Standard error of calibration	0.99%
Standard error of cross-validation	1.21%

## CONCLUSION

This application note demonstrates the feasibility of the DS2500 Liquid Analyzer for the determination of cannabinoid content in CBD oils. In comparison to the

HPLC method (**Table 3**), the time to result is a major advantage of NIR spectroscopy, since a single measurement is performed within one minute.

**Table 3.** Time to result for the cannabinoid content determination in CBD oils using HPLC method.

Parameter	Method	Time to result and workflow
Cannabinoid content	HPLC	5 min (preparation) + 40 min (HPLC)

## CONTACT

Metrohm Suisse SA  
Industriestrasse 13  
4800 Zofingen

[info@metrohm.ch](mailto:info@metrohm.ch)



### DS2500 Liquid Analyzer

Spectroscopie proche infrarouge robuste pour le contrôle qualité en laboratoire et en environnement de production.

L'analyseur DS2500 Liquid Analyzer est la solution éprouvée et souple destinée aux analyses de routine d'échantillons liquides, tout au long de la chaîne de fabrication. Sa conception robuste fait du DS2500 Liquid Analyzer un appareil insensible à la poussière, à l'humidité et aux vibrations, et donc particulièrement adapté aux rudes conditions d'un environnement de production.

Le DS2500 Liquid Analyzer couvre l'ensemble de la gamme spectrale de 400 à 2500 nm, chauffe les échantillons jusqu'à 80 °C et est compatible avec divers flacons à usage unique et cuves en quartz. Le 2500 Liquid Analyzer, lequel s'adapte à vos exigences individuelles en matière d'échantillons, vous permet d'obtenir des résultats précis et reproductibles en moins d'une minute. Avec sa détection du support d'échantillon intégrée et le logiciel Vision Air intuitif, un maniement simple et sûr est également garanti pour l'utilisateur.

En présence de grandes quantités d'échantillons, l'utilisation d'une cellule à flux continu associée à un robot passeur d'échantillons Metrohm peut augmenter considérablement la productivité.



### DS2500 - Support pour flacons à usage unique 8 mm

Support intelligent pour flacons en verre à usage unique de 8 mm de diamètre



## Vision Air 2.0 Complete

### Vision Air - logiciel universel de spectroscopie.

Vision Air Complete est une solution logicielle moderne et simple d'utilisation pour une application dans un environnement réglementé.

Aperçu des avantages de Vision Air :

- Des applications logicielles individuelles avec interface utilisateur adaptée sont le garant d'un maniement intuitif et simple
- Établissement et suivi simples des procédures de travail
- Base de données SQL pour une gestion sûre et simple des données

La version Vision Air Complete (66072208) comprend toutes les applications d'assurance qualité par spectroscopie Vis-NIR :

- Application de gestion des instruments et des données
- Application de développement de méthodes
- Application d'analyse de routine

Autres solutions Vision Air Complete :

- 66072207 (Vision Air Network Complete)
- 66072209 (Vision Air Pharma Complete)
- 66072210 (Vision Air Pharma Network Complete)