



Application Note AN-T-004

Chloride in meat products

Fully automated sample preparation and analysis based on ISO 1841-2

In order to maintain product quality, the sodium chloride content in meat products must be monitored, as the limit values defined by the respective public health authorities must not be exceeded. The chloride content in food correlates with the salt content; its determination is therefore described in various norms and standards. However, preparation of meat samples is time consuming, as it

requires homogenization with a mixer and a chloride extraction with water.

In order to reduce workload and increase sample throughput, this Application Note describes a fully automatic potentiometric titration of chloride with silver nitrate in meat products based on ISO 1841-2, including fully automated sample preparation using a Polytron homogenizer.

SAMPLE AND SAMPLE PREPARATION

The method is demonstrated for different meat products: pork sausage «Lyoner» and chicken breast with curry crust. If necessary, the spice crust around

the meat is removed and then the sample is cut into small pieces.

EXPERIMENTAL

This analysis is carried out on an automated system consisting of an OMNIS Advanced Titrator and an OMNIS Sample Robot S equipped with a dProfitrode and a dAg-Titrode. Furthermore, a Polytron homogenizer is used for sample preparation. Water is added to a reasonable and representative amount of sample. The pH is adjusted with nitric acid to below pH 1.5. The sample is titrated with standardized silver nitrate until after the equivalence point is reached. For dip rinsing of electrodes and burets, first water, then isopropanol is used. Afterwards, the electrodes are conditioned in water for one minute before the next sample.



Figure 1. OMNIS Sample Robot S, OMNIS Dosing Module and OMNIS Advanced Titrator equipped with dProfitrode and dAg-Titrode for the determination of chloride content.

RESULTS

The analysis demonstrates acceptable results and well-defined titration curves. The results and an

example titration curve are displayed in **Table 1** and **Figure 2**, respectively.

Table 1. Mean chloride content of two meat products determined with an automated OMNIS system (n = 6).

Sample	Chloride content in mg/100 g sample	SD(rel) in %
Pork sausage «Lyoner»	1175.5	1.1
Chicken breast with curry crust	1158.1	0.8

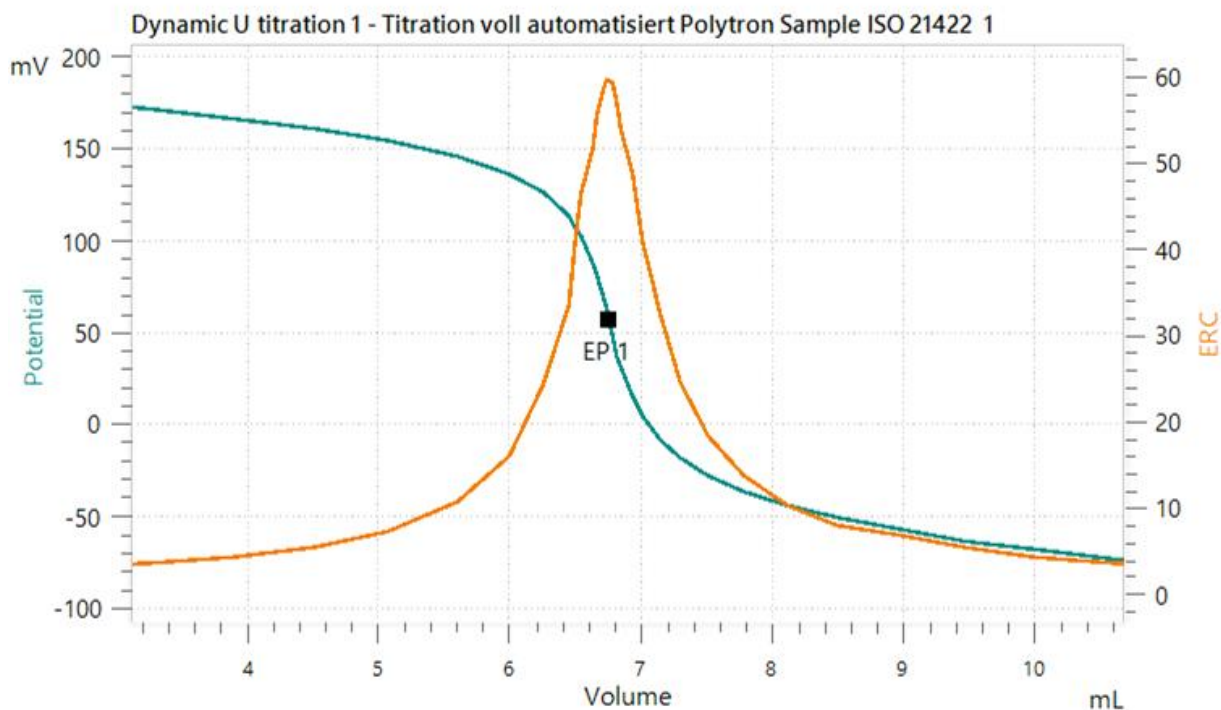


Figure 2. Example titration curve of the chloride determination of chicken breast.

CONCLUSION

Titration is a precise and reliable method to determine the chloride content in meat products according to international standards, such as ISO 1841-2. Using an OMNIS Sample Robot equipped with a Polytron homogenizer allows a fully automated sample preparation and chloride content determination of up

to four samples in parallel, increasing accuracy and freeing up valuable time of the operator and thus increasing the productivity in the lab. The OMNIS system offers the opportunity to customize the system according to your needs, and expand it for other required titration applications on foodstuff.

Internal reference: AW TI CH1-1264-112018

CONTACT

Metrohm France
13, avenue du Québec - CS
90038
91978 VILLEBON
COURTABOEUF CEDEX

info@metrohm.fr

CONFIGURATION



OMNIS Titrator Salt

L'OMNIS Titrator Salt vous offre un ensemble complet pour le titrage argentimétrique. Cet ensemble contient le titreur OMNIS Advanced Titrator avec un agitateur magnétique, une unité de cylindre de 10 mL, une d-AgTitrode pour le titrage avec du nitrate d'argent et le logiciel OMNIS Software avec une licence « standalone ».



Polytron PT 1300 D

Polytron PT 1300 D - version Metrohm

Homogénéisateur pouvant être commandé directement par le logiciel OMNIS, tiamo™ ou le Touch Control.

Le Polytron PT 1300 D se compose d'un module de contrôle et d'un moteur. Le système d'accouplement au moteur permet un remplacement facile et rapide des agrégats sans outils supplémentaires.

Les échantillons solides peuvent être fragmentés sans difficulté. Cet appareil est également idéal pour obtenir un bon mélange dans le cas d'échantillons visqueux.