



Application Note AN-PAN-1047

# Monitoring water content in refined products inline with NIR spectroscopy

Crude oil consists of at least 500 different components. It is processed by fractionation and refining to create many products including liquefied gas, gasoline, diesel, heating fuel, and lubricants. As per recent projections, the anticipated demand for crude oil is set to rise to 113 million barrels per day by 2025 [1].

This vital resource is used in many applications across various sectors. Crude oil is utilized during the manufacturing of plastics, textiles, dyes, cosmetics, fertilizers, detergents, building materials, and

pharmaceuticals.

This Application Note introduces a method for the «real-time» monitoring of water content in crude oil or refined products in refineries. To ensure safety, reliability, and optimal performance, a single explosion-proof inline process analyzer is recommended, such as the 2060 The NIR-Ex Analyzer by Metrohm Process Analytics. This minimizes human intervention, enhances product quality, and boosts profits, especially in the hazardous environment of a refinery.

In a refinery, crude oil is desalted then separated into several intermediate materials via an atmospheric or crude distillation unit (also known as a distillation tower or CDU), depending on its boiling temperature. The quality of fractions from the CDU must be continuously monitored.

To satisfy the high demand for gasoline, the heavier side cuts from the CDU are reformed and resolved to increase the light intermediate materials, thus increasing the gasoline fraction. The overhead distillate fraction naphtha (a mixture of C5 to C10 hydrocarbons) is produced from relatively light components and is supplied to ethylene plants as a raw material (**Figure 1**).


The CDU must operate efficiently at all times; however, the crude feed is full of impurities which cause corrosion and fouling throughout the refining process. Operating conditions that also influence corrosion and fouling include the temperature of the crude column overhead, crude, and reflux, as well as the water wash and overhead vapor water content.

Water extracts acids and amines present in the crude oil (see [AN-PAN-1001](#) for more information). This

vaporized water condenses as reflux liquid flowing down the column. The resulting heated salts are therefore deposited on the tower trays. These salts accumulate, causing a higher pressure drop, resulting in a loss of distillation column efficiency and profit.

Determining the water content in crude oil, refined petroleum products, fuels, biofuels, lubricants, and other related products is important for maintaining quality control, meeting trade specifications, protecting financial value, and enhancing process optimization. Monitoring this parameter enables the refinery to mitigate corrosion, safety problems, and infrastructure damage which can result from undesired moisture levels.

Generally, the determination of water content in naphtha fractions is performed with a reference method (i.e., Karl Fischer titration also provided by Metrohm) which requires several reagents. A safer, faster way to monitor the water content in CDU overhead fractions is inline with reagent-free near-infrared spectroscopy (NIRS). Spectroscopy offers numerous advantages over many wet-chemical analytical methods.

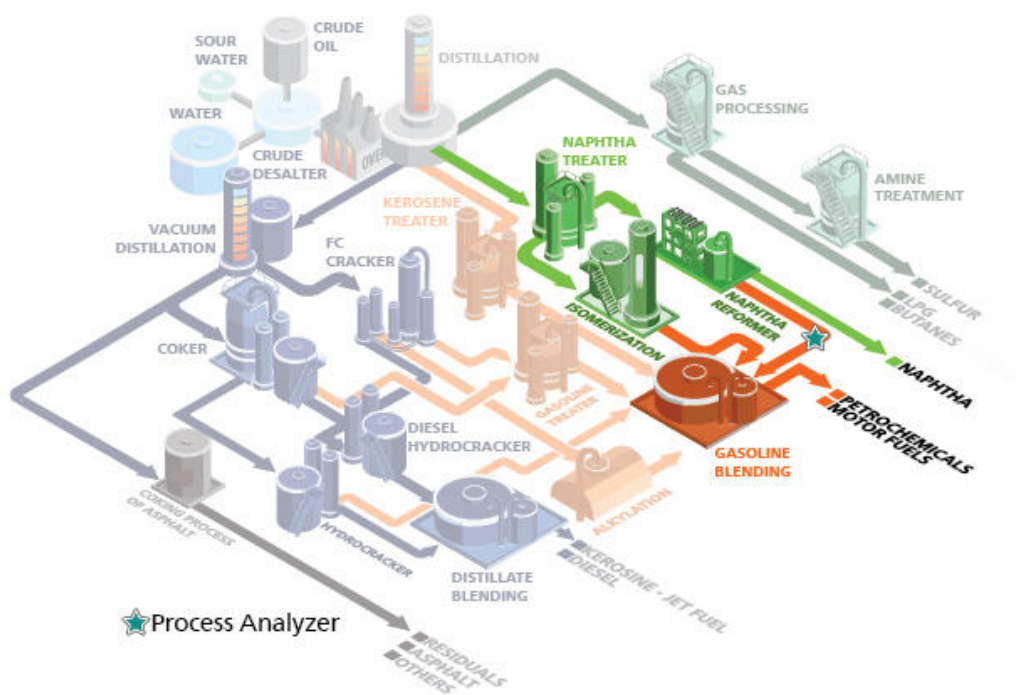

**Figure 1.** Illustration of the petrochemical refining process with a focus on the naphtha gas stream. The green star notes a suggested NIR measuring point.

## INTRODUCTION

Near-infrared spectroscopy is economical and fast, enabling qualitative and quantitative analyses that are noninvasive and nondestructive. A diverse range of parameters can be determined simultaneously in seconds from just one analysis. NIRS is an indispensable analysis technique that can be used along the entire production chain—from incoming materials to processing to the quality control of finished products.

Metrohm Process Analytics manufactures NIRS process analyzers that gather «real-time» spectral data from the process. These are used for comparison to a primary method (e.g., Karl Fischer titration) to create a simple, yet indispensable model to easily monitor QC parameters in near real-time. Gain more control over the refining process with a **2060 The NIR-Ex Analyzer** configured for applications in ATEX zones (Figure 2). This process analyzer is capable of monitoring up to five sample points per NIR cabinet with the multiplexer option.



**Figure 2.** The 2060 The NIR-Ex Analyzer from Metrohm Process Analytics is suitable for use in hazardous areas.

Each sample is measured in a 2 mm pathlength flow cell after the drying phase of naphtha. Wavelength


range used: 1800–2100 nm. An ATEX NIR process analyzer is recommended for explosion-proof areas.

**Table 1.** Typical concentration range of water content in naphtha fractions.

Components	Range (%)
Water	0–0.3

**TYPICAL RANGE**

Modeling and comparison to Primary Method:

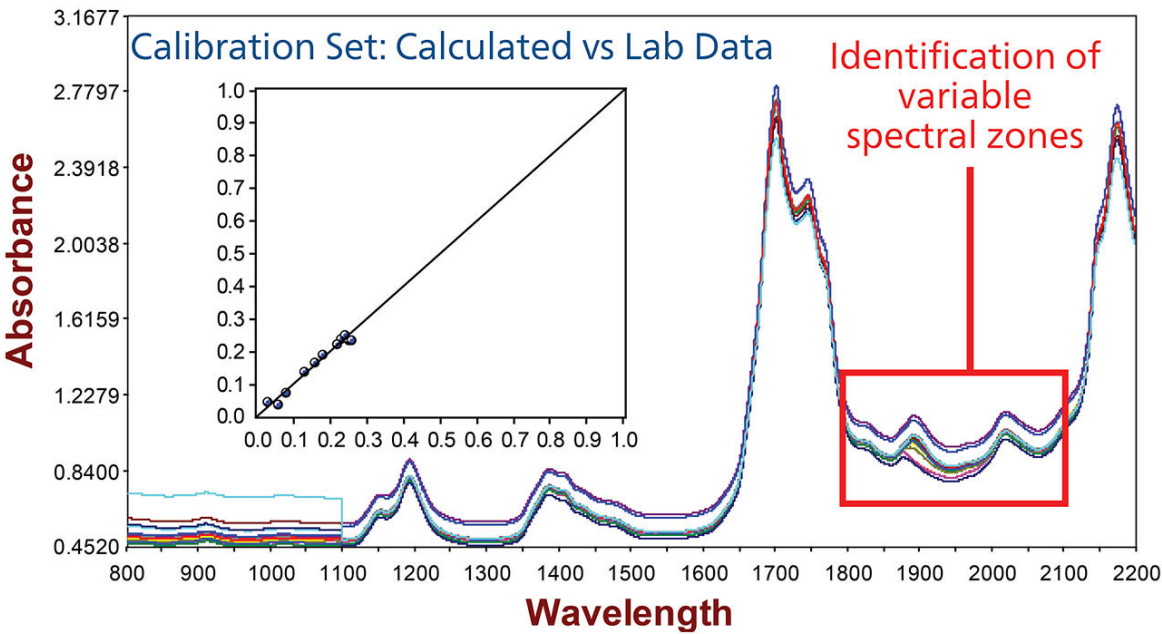

**Figure 3.** Data correlation between the primary method (Karl Fischer titration) and NIR spectra illustrating how accurate the correlation is between both methods.

A reference method (e.g., Karl Fischer titration) must still exist as a check method. An appropriate range of samples covering the process variability should be

analyzed by both methods to build an accurate NIR model. Correlations are made to specific process specifications.

Accurately monitoring water content in crude oil and its intermediate products in a refinery is of critical

importance. Impurities in the crude oil lead to corrosion and fouling, affecting operational efficiency.

The utilization of reagent-free NIRS provides a safer, faster, and noninvasive method for this purpose. Metrohm Process Analytics offers the 2060 *The* NIR-Ex Analyzer which is specifically designed for hazardous areas. This process analyzer is ideal for monitoring water content and other parameters in various

petrochemical products within seconds.

It is still recommended to maintain a reference method like Karl Fischer titration for verification purposes. Analyzing a range of samples with both methods is essential for building an accurate NIR model.

## RELATED PROCESS APPLICATION NOTES

[AN-PAN-1007](#) Online analysis of peroxide in the HP-PO process

[AN-NIR-025](#) Real-time inline predictions of jet fuel properties by NIRS

[AN-NIR-022](#) Quality Control of Gasoline – Rapid determination of RON, MON, AKI, aromatic content, and density

## OTHER RELATED DOCUMENTS

[8.000.5325](#) Water Content Analysis

## BENEFITS FOR NIR IN PROCESS

- Optimize product quality and increase profit with faster response time to process variations.
- Greater and faster return on investment.
- No manual sampling needed, thus less exposure of personnel to dangerous chemicals.
- Increase profits by reducing the occurrence of corrosion and fouling (i.e., controlled water content levels).

## BENEFITS FOR NIR IN PROCESS



## REFERENCE

1. *OPEC : Oil Outlook to 2025*.  
[https://www.opec.org/opec\\_web/en/1091.htm](https://www.opec.org/opec_web/en/1091.htm)  
(accessed 2023-10-16).



## CONTACT

Metrohm France  
13, avenue du Québec - CS  
90038  
91978 VILLEBON  
COURTABOEUF CEDEX

[info@metrohm.fr](mailto:info@metrohm.fr)

## CONFIGURATION



### 2060 The NIR-Ex Analyzer

Le **2060 The NIR-Ex Analyzer** est la nouvelle génération d'appareils de spectroscopie de processus de Metrohm Process Analytics. Avec sa conception unique et éprouvée de l'intérieur vers l'extérieur, il fournit des résultats précis toutes les *10 secondes*. Il peut fournir une analyse non destructive des liquides et des solides directement dans la ligne de traitement ou dans une cuve à réaction en utilisant des fibres optiques et des sondes de contact. Il a été conçu pour connecter jusqu'à cinq (5) sondes et/ou cellules à circulation. Chacun des cinq canaux peut être configuré indépendamment des autres à l'aide de notre logiciel propriétaire embarqué polyvalent.

De plus, cet appareil d'analyse est certifié IECEx et est conforme aux directives européennes ATEX. Il a été conçu avec un système de purge/pressurisation approuvé ainsi que des dispositifs intrinsèquement électroniques, empêchant toute fumée ou gaz potentiellement explosifs de l'air ambiant de pénétrer dans l'enceinte de l'appareil d'analyse. De plus, il est disponible en trois autres versions : le **2060 The NIR Analyzer**, **2060 The NIR-R Analyzer** et **2060 The NIR-REx Analyzer**.