

# Differentiation of inorganic salts using Raman spectroscopy

This Application Note shows the ability of handheld Raman systems like the Mira M-1 to identify and differentiate between salts such as carbonates, phosphates, and sulfates. The main focus of this work


was to evaluate the influence of the cationic part and the water of crystallization on the Raman-spectroscopic identification of the mentioned salts.

## INTRODUCTION

Inorganic salts often have the same anionic part, while the cationic part differs. Many salts can be distinguished by the number of water molecules bond to the salt.

In this study, the influences on the Raman spectrum of the cationic part of the salt and the number of water

molecules bound to its anionic part were investigated. Although the differences between the salts are very small, the spectra that were recorded using a handheld Raman spectrometer differed sufficiently to differentiate between them.

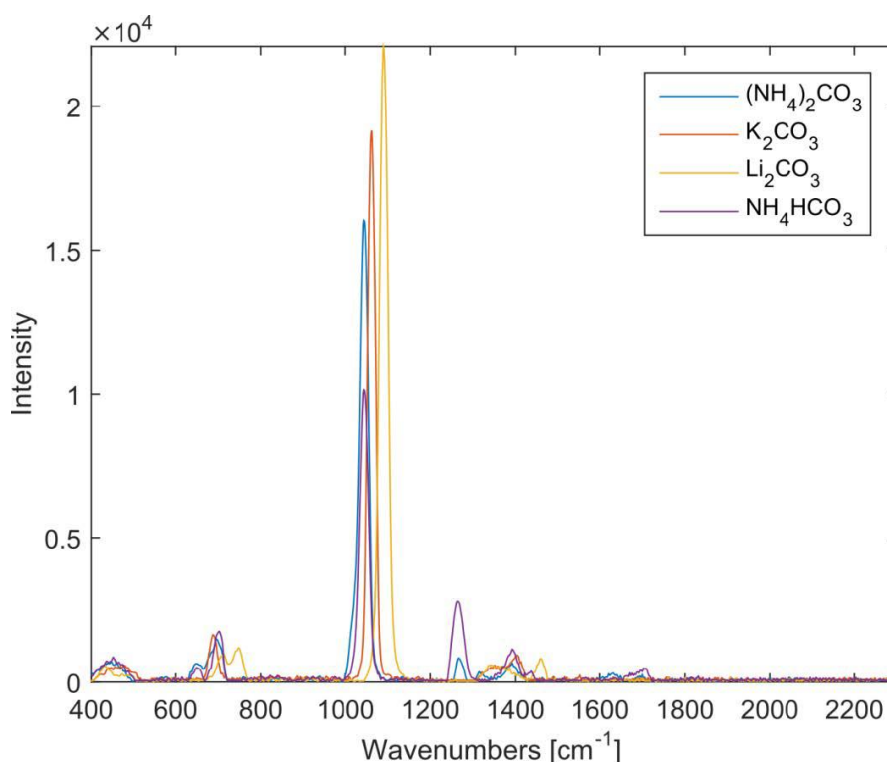

**Figure 1.** Overlaid Raman spectra of different carbonate salts.

## EXPERIMENTAL

All spectra were measured using the Mira M-1 Raman spectrometer in auto-acquisition mode, i.e., integration times were determined automatically. A laser wavelength of 785 nm and the Orbital-Raster-Scan (ORS) technique were used. The samples were

analyzed in small vials with the vial holder adapter. Three different anions that give are Raman-active were chosen: carbonate, phosphate, and sulfate. The cationic part of the salts was varied and the resulting spectral changes were investigated.

## RESULTS AND DISCUSSION

Figure 2 shows how the carbonate peak in the Raman spectrum shifts depending on the counter cation. This shift is significant enough to use it to differentiate between the various carbonate salts (except for ammonium carbonate and ammonium bicarbonate, where the difference is very small).


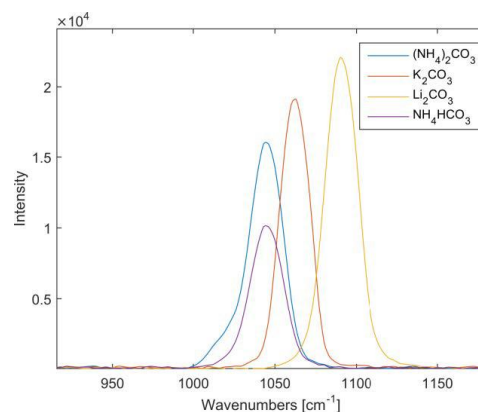


Figure 2. Main peaks of the various carbonates.

Similar results are also observed for various phosphates; the differences in the spectra are useful for their differentiation (see Figure 3) – despite the fact that there are some difficulties when trying to


distinguish between diammonium phosphate and dipotassium phosphate (due to the similar ionic radius of potassium and ammonium).

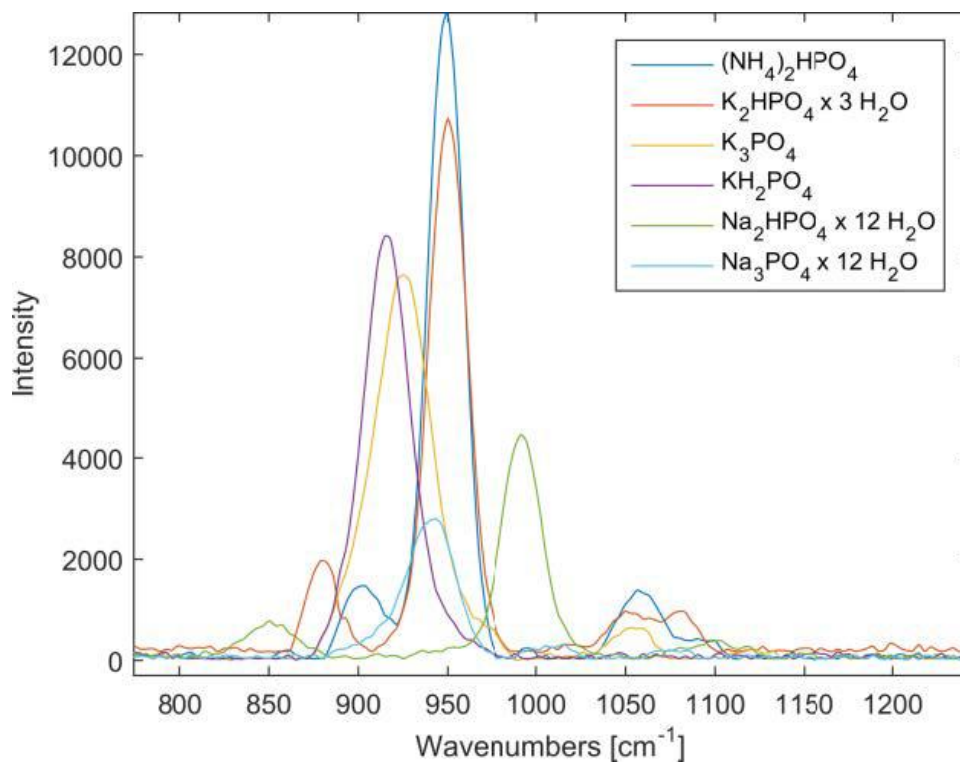

**Figure 3.** Main differences in the spectra of the phosphates.

The analyzed sulfates also differed from each other significantly, allowing their unambiguous identification with the handheld Mira M-1 (see **Figure**

**4**), although  $\text{CuSO}_4 \times 7 \text{H}_2\text{O}$ ,  $\text{K}_2\text{SO}_4$ ,  $\text{SnSO}_4$ , and  $\text{ZnSO}_4 \times 7 \text{H}_2\text{O}$  could not be identified unambiguously due to their similar spectra.

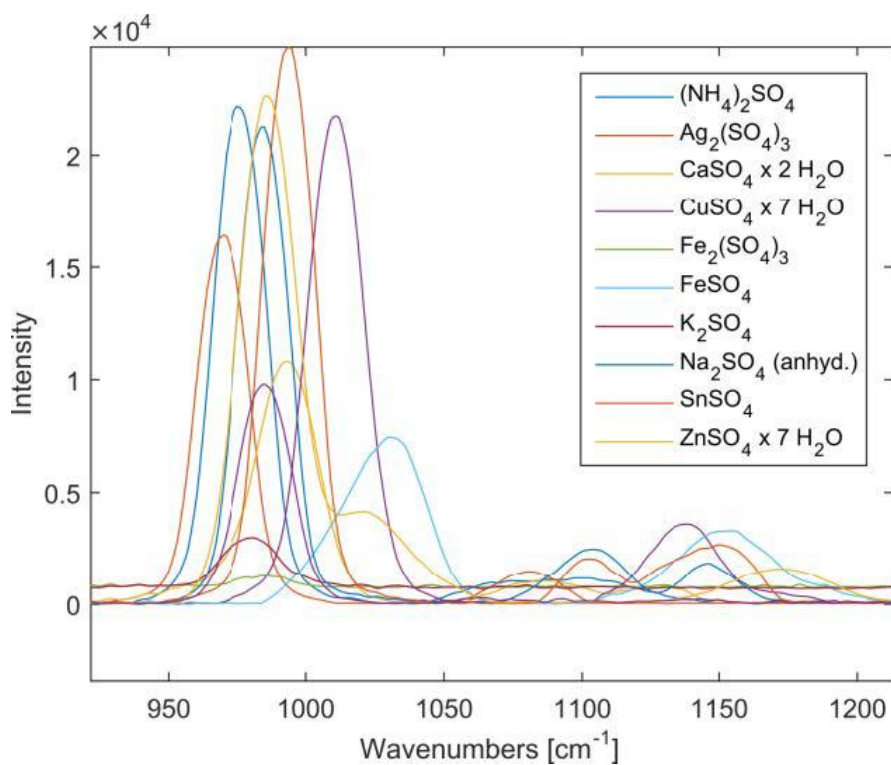

**Figure 4.** Main differences in the spectra of the sulfates.

## CONCLUSIONS

Generally speaking, handheld Raman spectrometers, such as the Mira M-1, are very useful when it comes to inorganic material identification, even when dealing with salts having the same anionic part. Differences in

the cationic parts of the salts help to unambiguously identify many salts with the Mira M-1 handheld Raman analyzer.

## CONTACT

Metrohm France  
 13, avenue du Québec - CS  
 90038  
 91978 VILLEBON  
 COURTABOEUF CEDEX

[info@metrohm.fr](mailto:info@metrohm.fr)

## CONFIGURATION



### MIRA P Advanced

Le Metrohm Instant Raman Analyzer (MIRA) P est un spectromètre Raman portable performant qui s'utilise pour les déterminations rapides et non destructives et le contrôle des matériaux les plus divers, comme les principes actifs pharmaceutiques et les excipients. De très petite taille, le MIRA P est pourtant très robuste et dispose d'une structure de spectrographe haute efficacité, équipée de notre technologie « Orbital Raster Scan » (ORS) inédite. MIRA P satisfait aux prescriptions FDA 21 CFR partie 11.

Le Advanced Package comprend une lentille avec laquelle les matériaux peuvent être analysés directement ou dans leur conditionnement (classe de laser 3b), ainsi qu'un support de flacon pour analyser les échantillons dans des flacons en verre (classe de laser 1).