



Application Note AN-EC-028

Measuring hydrogen permeation according to ASTM G148

How VIONIC powered by INTELLO can be used to study hydrogen permeation

In aqueous solution, hydrogen atoms are produced on the sample surface by electrochemical reactions. Hydrogen formation is encountered in different situations including electroplating, corrosion, and cathodic protection. The hydrogen atoms formed can permeate inside the sample material and accumulate in defective sites, causing cracks, inducing corrosion, and diminishing the mechanical properties of the

sample.

It is therefore important to measure the hydrogen permeation in samples by studying hydrogen evolution and successive diffusion in samples.

In this Application Note, hydrogen permeation experiments are conducted following the procedure described in the ASTM standard G148.

EXPERIMENTAL SETUP

The experiment was carried out in a H-cell composed of two chambers separated by the working electrode shared between the compartments.

In one side (i.e., the «charging side»), hydrogen is formed at the working electrode surface. The

hydrogen is detected in the other side (i.e., «oxidation side» or «detection side») [1].

The hydrogen permeation experiment was conducted with two VIONIC powered by INTELLO instruments from Metrohm Autolab (Figure 1).



Figure 1. VIONIC powered by INTELLO.

Since both instruments shared the same working electrode, they were set in floating mode – working electrode grounded. The working electrode was not physically connected to the ground.

One instrument was used to produce hydrogen on the sample by applying a negative current in galvanostatic mode. The other instrument was used in potentiostatic mode to oxidize the permeated hydrogen and to measure the resulting permeation current.

The working electrode was a 316L stainless steel foil of 50 μm thickness. The area exposed to each side of the H-cell was 1.8 cm^2 . The charging side was filled with an acidic solution composed of 1 mol/L HCl in deionized water, where 0.25 g/L of disodium hydrogen arsenate heptahydrate ($\text{Na}_2\text{HAsO}_4 \cdot 7\text{H}_2\text{O}$) was added to promote the hydrogen formation and permeation [2]. A Metrohm PT.SHEET was used as counter electrode. No reference electrode was used.

The oxidation side was filled with an aqueous solution of 0.1 mol/L NaOH (alkaline solution). A Metrohm Ag/AgCl 3 mol/L KCl reference electrode and a Metrohm PT.SHEET platinum electrode were used as reference and counter electrode, respectively. None of the solutions were deaerated.

The procedures consisted of the following steps:

1. The alkaline solution is added to the oxidation cell, together with the electrodes.

2. The procedure to detect hydrogen is started at the oxidation cell. In potentiostatic mode, +300 mV vs. OCP (open circuit potential) is applied. The recorded current decreases due to the relaxation of the polarization.
3. When the oxidation current is stable, the acidic solution is added to the charging side of the cell and the charging procedure is started. In galvanostatic mode, a negative (reductive) current of -1 mA/cm² is applied to the working electrode. In this experiment, a current of -1.8 mA was applied.

RESULTS AND DISCUSSION

Figure 2 shows the plot of oxidation current vs. time which is related to the polarization in the oxidation

side.

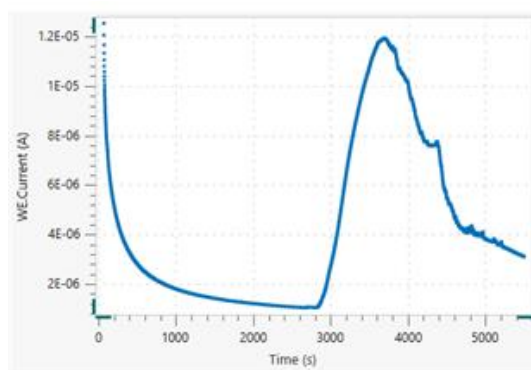


Figure 2. Plot showing oxidation current vs. time.

At the beginning of the recording, the current decreases due to the relaxation of polarization. The polarization is induced by applying 300 mV vs. OCP to the working electrode.

At approximately 2700 s, a small bump in the graph is visible. At that time, the charging side was filled up

with the acidic solution and the production of hydrogen started.

The hydrogen permeation started to be detected at approximately 2800 s. Here, the current increased again due to the hydrogen becoming oxidized at the detection side.

CONCLUSIONS

In this Application Note, the study of hydrogen permeation according to ASTM G148 across a 316L stainless steel sample was presented.

This work was possible with the use of two VIONIC powered by INTELLO instruments, both in floating mode – working electrode grounded.

An H-cell was used for this study where the working

electrode was shared between two compartments. One side was used to generate hydrogen with an acidic solution, and the other side was used to detect hydrogen with an alkaline solution.

The hydrogen permeation was triggered using disodium hydrogen arsenate heptahydrate, added in the acidic solution.

REFERENCES

1. ASTM G148 - Standard Practice for Evaluation of Hydrogen Uptake, Permeation, and Transport in Metals by an Electrochemical Technique.
2. Charca, S. M. Study of Hydrogen Permeation and Diffusion in Steels: Predictive Model for Determination of Desorbed Hydrogen Concentration - ProQuest, University of Puerto Rico, Mayaguez, 2006.

FOR MORE INFORMATION

More information about this Application Note and the associated INTELLO software procedure is available from your local Metrohm distributor. Additional

instrument specification information can be found at: www.metrohm.com/en/products/electrochemistry

CONTACT

Metrohm Italiana Srl
Via G. Di Vittorio, 5
21040 Origgio (VA)

info@metrohm.it

CONFIGURATION



VIONIC

VIONIC è il nostro potenziostato/galvanostato di nuova generazione, con il nuovo software di Autolab INTELLO.

VIONIC offre la **combinazione di caratteristiche tecniche più versatile di qualsiasi altro strumento singolo** disponibile al momento sul mercato.

- Tensione conforme: ± 50 V
- Corrente standard ± 6 A
- Frequenza EIS: fino a 10 MHz
- Intervallo di campionatura fino a 1 μ s

Nel prezzo di **VIONIC** sono incluse anche funzioni che normalmente rappresenterebbero un costo aggiuntivo con la maggior parte degli altri strumenti quali ad esempio:

- Spettroscopia di impedenza elettrochimica (EIS)
- Modalità flottante selezionabile
- Secondo elettrodo di rilevamento (S2)
- Scansione analogica



Elettrodo a foglio di platino

Questo elettrodo è costituito da un foglio sottile di platino incorporato in uno stelo in vetro. Questo elettrodo può essere usato come controelettrodo per la maggior parte di misure elettrochimiche. La superficie è di circa 1 cm².



Elettrodo di riferimento Ag/AgCl

Elettrodo di riferimento argento/cloruro di argento con $c(\text{KCl}) = 3 \text{ mol/L}$ come elettrolita di riferimento. Questo elettrodo di riferimento è adatto alle applicazioni acquose e il giunto conico 14/15 consente uno smontaggio semplice.