



Application Note AN-PAN-1014

Online determination of salt in crude oil by automated process analysis

Crude oil is a highly complex mixture of hydrocarbons which contains different organic and inorganic impurities (e.g., water and inorganic salts). Excessive amounts of salt in crude oil results in higher corrosion rates in refining units and has a detrimental effect on the catalysts used. Therefore, salt needs to be removed from crude oils prior to refining, in a process known as desalting.

Desalting techniques are well established, but continuous monitoring of the salt content in

crude oil is needed for process control and cost reduction.

This Process Application Note is focused on monitoring the salt content in crude oil using the ADI 2045TI Ex proof Analyzer from Metrohm Process Analytics equipped with special heavy-duty sampling devices. This online analysis solution ensures a safe working environment for operators, avoids corrosion from excess salt in crude, and increases profitability of the desalting process.

INTRODUCTION

Crude oil is extracted from wells which contain water, gases, and inorganic salts (either dissolved or suspended). These salts can lead to downstream fouling and corrosion of heat exchangers and distillation overhead systems. Furthermore, salts are detrimental for catalysts in the downstream conversion processes.

Salt is removed from crude oil via two major methods: chemical and electrostatic separation. The most commonly applied method is **electrical desalting** [1]. Both of these methods use hot water as the extraction agent.

Excess water has to be removed first, therefore desalting takes place before distillation. After preheating to 115–150 °C, the oily feedstock is mixed with water in order to dissolve and wash out the salts. The water must then be separated from the oil feedstock in a separating vessel by adding demulsifier chemicals to break up the emulsion and in addition, by applying a high-

potential electric field (via electrostatic grids) across the settling vessel to coalesce the polar saltwater droplets (**Figure 1b**). The wash water (brine) containing dissolved hydrocarbons, free oil, dissolved salts, and suspended solids, is treated further in an effluent treatment plant. Efforts are made in the industry to reduce water content of the desalted crude to less than 0.3%.

Traditionally, the desalting process (**Figure 1a**) can be monitored by laboratory pH analysis. This method helps to determine the speed of phase separation between the two phases (water-oil). However, this methodology does not provide timely results and requires human intervention to implement the laboratory analysis results into the process. Online process analysis allows constant monitoring of crude oil quality without long waiting times in the laboratory, providing more accurate and representative results directly to the control room.

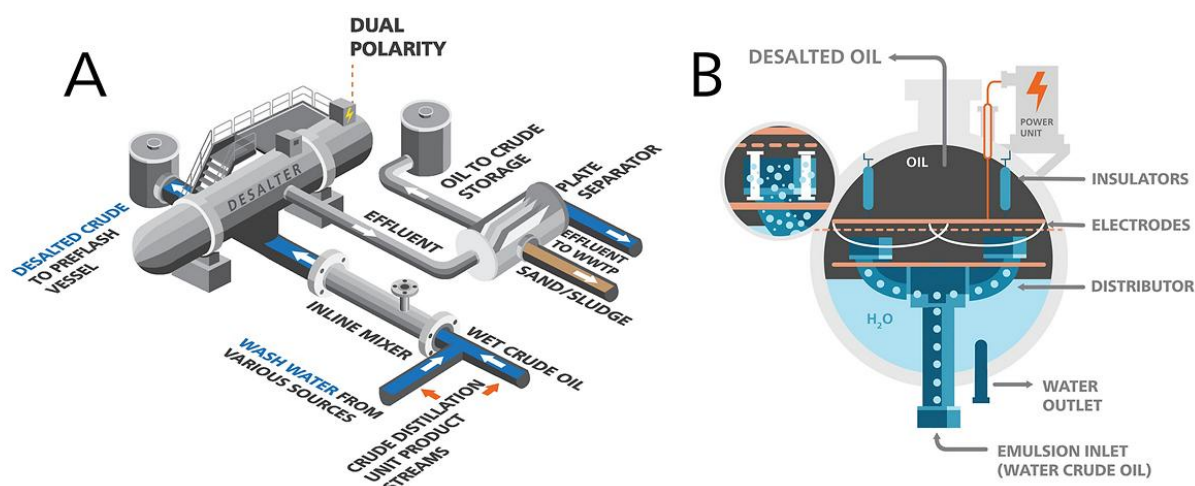


Figure 1. (a) Schematic diagram of a typical crude oil desalter process. (b) Cross-sectional view of a crude oil desalter.

Additionally, testing of crude and refined oil products is demanding and requires precise and reliable analysis to meet regulatory demands. Metrohm Process Analytics is actively involved with international standard bodies to help drive

method development. The **ADI 2045TI Ex proof Analyzer** (**Figure 2**) can monitor chloride in the crude after desalting according to ASTM D3230 testing procedures.

APPLICATION

Chloride is analyzed with conductivity detection as described in ASTM D3230 with the ADI 2045TI Ex proof Analyzer (**Figure 2**).



Figure 2. ADI 2045TI Ex proof (ATEX) Analyzer.

Table 1. Typical chloride concentration range in crude oil according to ASTM guidelines

Components	Range (mg/kg)
Chloride	0–500

CONCLUSION

Monitoring the chloride in crude oil before and after the desalting process is necessary to check the process efficiency and to overcome corrosion problems downstream. Since the sample take-off point is typically located in a hazardous

environment, the ADI 2045TI Ex proof Analyzer is designed and equipped to meet directive 94/9EC (ATEX95). No «hot work permits» are needed for maintenance and the analyzer can be remotely controlled.

REMARKS

Other measurement techniques can apply for low economy grade crudes like the Standard Test Method for Salt in Crude Oils (Potentiometric Method) ASTM D6470. Karl

Fischer titration can be applied for moisture/water content determination as an additional parameter in the desalter.

RELATED ASTM METHODS

- ASTM D3230: Standard Test Method for Salts in Crude Oil (Electrometric Method)

- ASTM D6470: Standard Test Method for Salt in Crude Oils (Potentiometric Method)

RELATED APPLICATION NOTES

AN-PAN-1001 Hydrogen sulfide and ammonia in sour water

AN-PAN-1026 Mercaptans and hydrogen sulfide in raw oil in accordance with ASTM D3227 and

UOP163

AN-PAN-1047 Inline monitoring of water content in naphtha fractions by NIRS

BENEFITS FOR ONLINE DESALTING ANALYSIS

- No «hot work permits» are needed for maintenance, and the analyzer can be remotely controlled
- **Safe production** due to near «real-time» monitoring and no exposure of operator to chemical reagents
- Greater and faster **return on investment (ROI)**
- **More savings** per measurement, making results more cost-effective
- **Increased product throughput**, reproducibility, production rates, and profitability



REFERENCE

1. Al-Otaibi, M. B.; Elkamel, A.; Nassehi, V.; Abdul-Wahab, S. A. A Computational Intelligence Based Approach for the Analysis and Optimization of a Crude Oil Desalting and Dehydration Process. *Energy Fuels* **2005**, *19* (6),2526–2534.
<https://doi.org/10.1021/ef050132j>.

CONTACT

メトロームジャパン株式会社
143-0006 東京都大田区平和島6-1-1
null 東京流通センター アネックス9階

metrohm.jp@metrohm.jp

CONFIGURATION



ADI 2045TI Ex proof Analyzer

ADI 2045TI Ex 防爆型プロセスアナライザーは、防爆仕様が決定的重要性を持つ安全要求事項となるような危険な地域で使用されます。この装置はEU規定94/9/EG (ATEX95)を満たし、爆発の恐れのあるゾーンIおよびIIでの使用が認可されています。その構造は、空気清浄システムおよび過圧システムをそれに属する電子安全装置と組み合わせたものであります。空気清浄工程および持続的な過圧により、爆発性雰囲気内で空気が分析装置のハウジングに侵入するのを防ぎます。分析装置のインテリシエントな構造により、大型の分析装置保護設備の洗浄は不要で、また危険区域内にある製品ラインへの装置設置が可能となります。

滴定、カールフィッシャー滴定、測光法、イオン選択性電極による測定と並んで、このEx-pバージョンによる直接測定も可能です。