

Identification of monomers with Raman spectroscopy

Polymers are comprised of macromolecules that are in turn comprised of numerous identical or similar structural units that are referred to as monomers. This Application Note shows the convenient identification of conventional monomers within seconds using the portable Mira M-1 spectrometer. Monomers such as

styrol, various alkyl methacrylates, divinylbenzene, ethylene glycol, phenol, terephthalic acid and urea have been investigated. Additives or inhibitors such as benzoquinone can be identified quickly and unambiguously.

INTRODUCTION

Today's industry, but also daily life, cannot be imagined without polymers. With the variety of the available polymers on the market, the number of monomers and especially additives, used to endow the polymers with special properties, is enormous.

Many polymer manufacturers, if not all, use their own special mixtures and additives, commonly carrying proper names, making it hard to get an idea of the

function of certain additives. Nevertheless, all use the same monomers, which also means, that every polymer manufacturer will profit from a quick raw material check before feeding the raw materials into their polymerization process.

In this study, a library of commonly used monomers was built and subsequently used for the identification of unknown monomers.

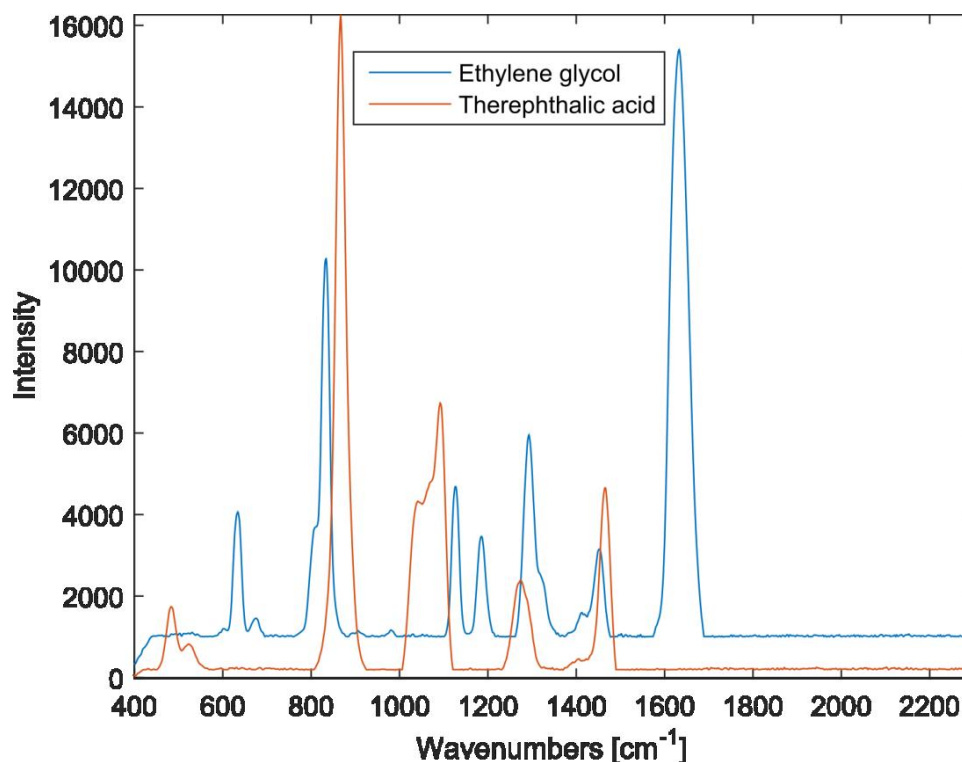


Figure 1. Raman spectra of ethylene glycol and terephthalic acid

EXPERIMENTAL

All spectra were measured using the Mira M-1 handheld Raman spectrometer in auto-acquisition mode, i.e. integration times were determined automatically. A laser wavelength of 785 nm and the Orbital-Raster-Scan (ORS) technique were used. Some

of the monomers were filled into vials and analyzed using the vial holder attachment, while other samples were analyzed directly in their plastic container using the long working distance (LWD) lens.

The following monomers were used in this study:

Monomer	Meas. mode	Usage
Divinylbenzene (DVB)	LWD	Styrene-DVB Copolymer (S-DVB)
Ethylene glycol	vial	Polyethylene terephthalate (PET)
Ethyl methacrylate	vial/LW	Paraloid B-72 (thermoplastic resin used for surface coatings and conservations)
Formaldehyde	vial	Polyoxymethylene (POM), Bakelite, urea-formaldehyde (UF), melamine-formaldehyde (MF)
Urea	vial	Urea-formaldehyde (UF)
Hexamethylenetetramine (HMTA)	vial	Hardening component for phenolic resins

Hydroquinone	vial	Polyether ether ketone (PEEK)
Methyl methacrylate (MMA)	LWD	Poly(methyl methacrylate) (PMMA)
Phenol	vial	Bisphenol-A (a precursor to polycarbonates and epoxide resins)
Styrene	vial	Polystyrene (PS), S-DVB
Therephthalic acid	vial	Polyethylene terephthalate (PET)

RESULTS AND DISCUSSION

To build the library, the samples were measured in vials but also with the LWD lens through amber bottles. Using the Mira Cal software, the spectra were

investigated to check for visible differences between the monomers. **Figure 2** shows an overlay of all the analyzed monomers.

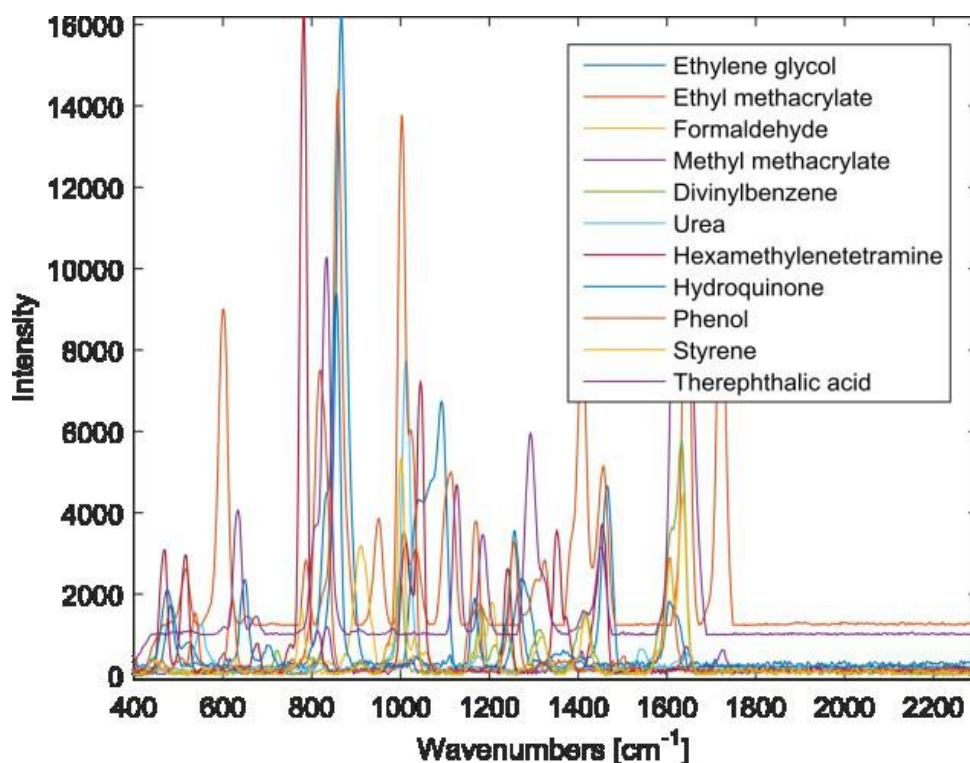


Figure 2. Overlay of the analysed monomers.

When using Mira in its autonomous mode, i.e., mode, without the use of the Mira Cal software, secure

identification of the monomers was achieved, and the correlation coefficients were always greater 0.95.

CONCLUSIONS

This study shows that Mira M-1 can be used to unambiguously identify polymer raw materials used to produce commonly used polymers such as PET, POM and PEEK by measuring their spectra and

matching them with a library. The identification takes just a few seconds. Additionally, additives or inhibitors such as benzoquinone can be quickly and unambiguously identified.

CONTACT

Metrohm Viet Nam
Phan Dinh Giot
70000 Ho Chi Minh

info@metrohm.vn

CONFIGURATION



MIRA P Advanced

The Metrohm Instant Raman Analyzer (MIRA) P is a high-performance, handheld Raman spectrometer used for rapid, nondestructive determination and verification of different material types, such as Pharmaceutical APIs and excipients. Despite the small size of the instrument, the MIRA P has a ruggedized design and features a high-efficiency spectrograph design equipped with our unique Orbital-Raster-Scan (ORS) technology. The MIRA P is fully compliant with FDA 21 CFR Part 11 regulations.

The Advanced Package includes an attachment lens for analyzing materials directly or through containers (laser class 3b), as well as a vial holder attachment for analyzing samples contained in glass vials (laser class 1).