



Application Note AN-T-025

Hydrogen peroxide content in aqueous solutions

Reliable and inexpensive determination according to ASTM D2180

Peroxides are often used for disinfection and water treatment purposes due to their antiseptic properties. Lower concentrations between 0.3–3% are used in households, while higher concentrations can be used for sterilization purposes.

Additionally, peroxides are utilized as oxidizing and bleaching agents. They are used for pulp and paper bleaching, as well as a mild whitener in laundry detergents and some cosmetic dental products.

Peroxides, perborates, and percarbonates can easily be determined by titration. This application note presents two titration methods for peroxide analysis. The first method is performed according to **ASTM D2180**, and is suitable for samples such as bleaching components or concentrated hydrogen peroxide solutions. The second method for the determination of traces of hydrogen peroxide is suitable for aqueous samples with concentrations as low as 0.4 mg/L.

SAMPLE AND SAMPLE PREPARATION

This application study is demonstrated on aqueous solutions containing various hydrogen peroxide concentrations ranging from 0.4 mg/L to 32%.

Samples with traces of H_2O_2 do not require any sample preparation. Samples with higher

concentrations are diluted with deionized water. Both sample size and dilution factor should be chosen depending on the expected peroxide content. Ideally, an aliquot of the diluted sample results in an equivalence point of approximately 10 mL.

EXPERIMENTAL

The analysis is performed on an OMNIS Advanced Titrator equipped with a combined Pt ring electrode according to **ASTM D2180**. Before titration, the sample is acidified with sulfuric acid. In case of trace amounts, the sulfuric acid is modified to contain manganese sulfate as a catalyst. This modification allows a lower

method detection limit.

Samples are titrated with potassium permanganate until after the equivalence point is reached. For samples with trace amounts of hydrogen peroxides, a lower titrant concentration is used.

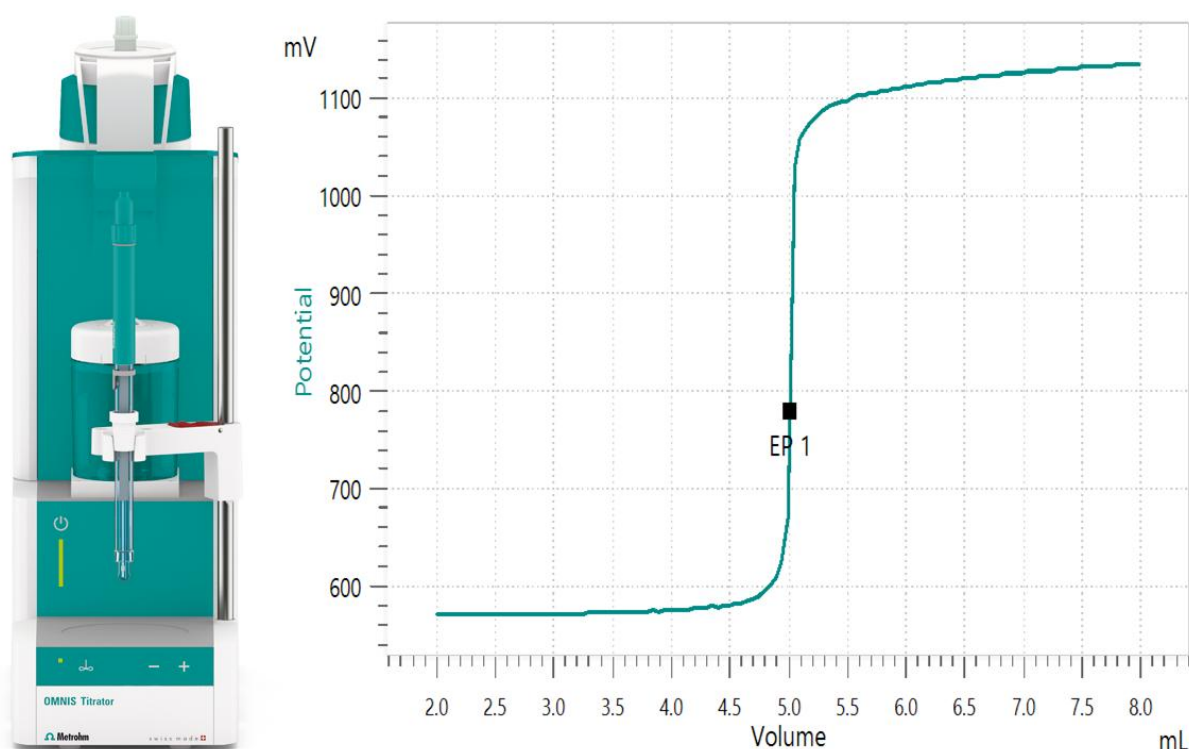


Figure 1. OMNIS Advanced Titrator and an example titration curve. (Left) OMNIS Advanced Titrator equipped with a digital Pt ring electrode for the determination of peroxides in aqueous solutions. (Right) A titration curve is displayed of sample no. 2 (Table 1) titrated according to ASTM D2180.

RESULTS

Sharp titration curves with a large potential difference are obtained for all tested samples

and with both methods. This results in reproducible results as displayed in **Table 1**.

Table 1. Results of the peroxide determination in various aqueous solutions. Samples 1 and 2 are determined according to ASTM D2180, while samples 3 and 4 are determined according the modified method for trace amounts of peroxides.

No	n	Mean value	SD(abs)	SD(rel)
1	8	32.14%	0.03%	0.09%
2	3	85.82 mg/L	0.83 mg/L	0.97%
3	3	4.27 mg/L	0.01 mg/L	0.23%
4	5	0.40 mg/L	0.01 mg/L	2.50%

CONCLUSION

Titration is a fast and inexpensive method, allowing reliable determination of peroxides in aqueous solutions according to **ASTM D2180**. A modified method for trace concentrations permits accurate and reproducible peroxide determinations as low as 0.4 mg/L. State-of-the-art OMNIS Titrators from Metrohm

provide a whole new level of titration. The modular design of OMNIS Titrators offers complete application flexibility. The system can be expanded whenever necessary, allowing growth over time. With a resolution of 100,000 steps, maximum dosing accuracy can be achieved, further improving reproducibility.

Internal references: AW TI CH1-1296-012020;

AW TI CH1-0350-0187

CONTACT

瑞士万通中国
北京市海淀区上地路1号院
1号楼7702
100085 北京

marketing@metrohm.com.cn

CONFIGURATION



OMNIS Advanced Titrator

新型、模式位分析 OMNIS Titrator 滴定,于独立行或作 OMNIS 滴定系的核心元件行,用于使用 OMNIS Sample Robot 行点和等当点滴定(一/)。由于采用 3S 瓶配器技,理化学品从未像在一安全。可以使用量模和量管元自由配置滴定,并在需要展一台螺旋拌器。在需要可以通相的件功能可平行滴定升 OMNIS Advanced Titrator。

- 通算机或本地网控制
- 可以其他用或助溶液外接最多四个滴定模或加液模
- 螺旋拌器的接方式
- 可提供不同大小的量管:5、10、20 或 50 mL
- 采用 3S 技的瓶配器:安全理化学品,自生商的原
始数据

量模式和件:

- 点定滴定:“Basic” 功能可
- 点和等当点滴定(一/):“Advanced” 功能可
- 点和等当点滴定(一/),包括平行滴定
:“Professional” 功能可



dPt Titrode

pH 玻璃膜的 OMNIS 用数字合式形,用作参比。
免用于 pH 恒定的化原滴定,例如:

- 量法
- 重酸法
- 量法
- 高酸滴定法

存放在蒸水中。

dTodes 可在 OMNIS Titratoren 上使用。