



Application Note AN-T-213

水中的臭

Easy determination of ozone in water

Water treatment with ozone (O_3) is a common procedure for the disinfection of swimming pools. To efficiently kill microbes, ozone concentrations from 0.1–7 mg min/L are needed. During this process, it is important that a sufficient but not excessive amount of O_3 is produced to disinfect the water. Otherwise, the remaining ozone which is not used to disinfect the water could enter the swimming water. This concentration should not exceed 0.04 mg/L. If the concentration is higher, the ozone could irritate the respiratory system or the skin of bathers.

Therefore, it is recommended to monitor the produced ozone concentration. In addition, the disinfection process with ozone is used in drinking and waste water treatment. This is due to the fact that ozone is significantly more effective than chlorine at inactivating or killing viruses and bacteria. Ozone is widely used in Europe to treat drinking water.

This application note describes a method to determine the ozone concentration in water by potentiometric titration according to DIN 38408-3.

SAMPLE AND SAMPLE PREPARATION

Due to the reactive nature of ozone, this application is demonstrated on spiked groundwater. Immediately after spiking the

sample with ozone (produced by electrolysis), potassium iodide solution is added to the sample to stabilize the ozone.

EXPERIMENTAL

This analysis is performed on an OMNIS Advanced Titrator equipped with a double Pt sheet electrode.

Sulfuric acid is added to a prepared sample solution, and the iodine, generated by the reaction of ozone with potassium iodide, is back titrated with sodium thiosulfate until after the equivalence point.

It is important to determine the ozone content immediately after the sample is prepared, because the ozone is not stable.



Figure 1. OMNIS Advanced Titrator equipped with a double Pt sheet electrode for the determination of ozone in water samples.

RESULTS

A mean ozone content of 13.44 mg/L ($n = 3$, $SD(abs) = 0.83$ mg/L, $SD(rel) = 6.18\%$) is obtained for the spiked groundwater sample. If ozone is not generated in-situ but continuously, it should be possible to obtain a lower standard

deviation.

With the used setup and titration parameters, one sample could be measured in under 2.5 minutes with sharp curves and clear equivalence points.

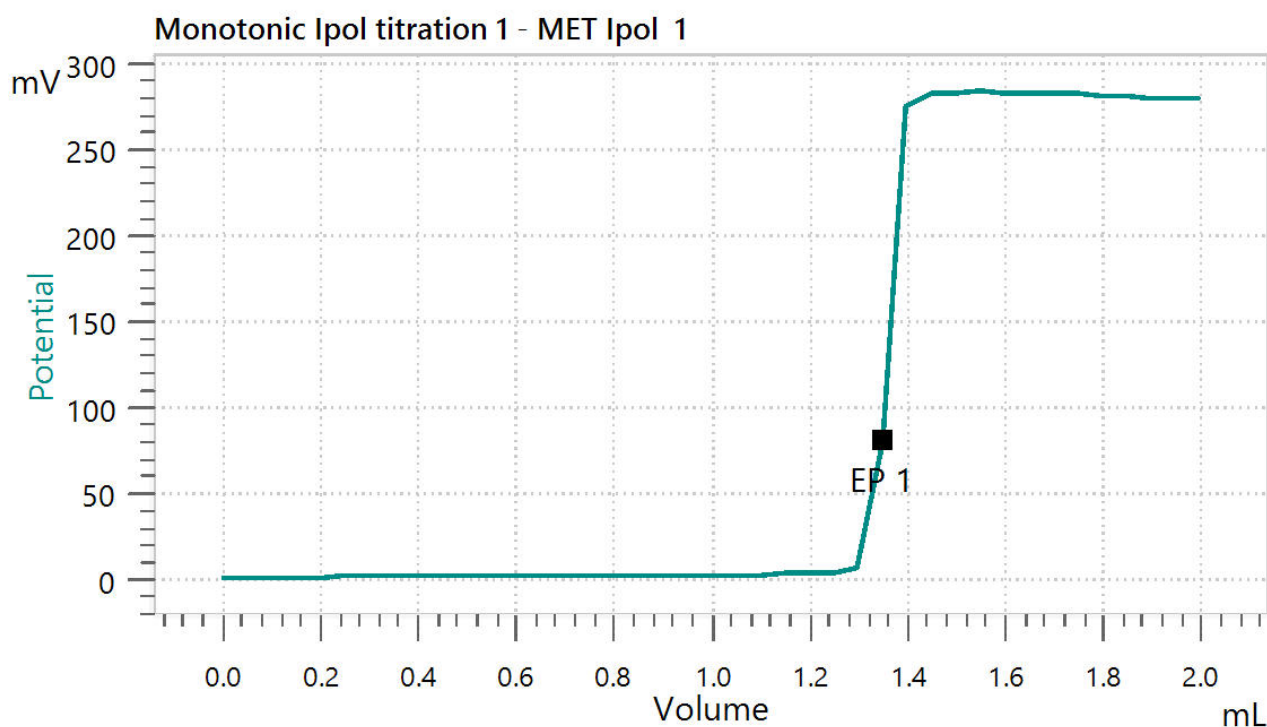


Figure 2. Example titration curve of the ozone determination in spiked groundwater.

CONCLUSION

Titration is an inexpensive method to determine ozone in water. With this method, it is possible to determine ozone contents as low as 0.1 mg/L.

Using an OMNIS Titrator allows you to customize the

system according to your application needs and to expand it for other titration applications required for the quality control of water.

Internal reference: AW TI CH1-1297-012020

CONTACT

瑞士万通中国
北京市海淀区上地路1号院
1号楼7702
100085 北京

marketing@metrohm.co
m.cn

CONFIGURATION



OMNIS Advanced Titrator

新型、模式位分析 OMNIS Titrator 滴定,于独立行或作 OMNIS 滴定系的核心元件行,用于使用 OMNIS Sample Robot 行点和等当点滴定(一/)。由于采用 3S 瓶配器技,理化学品很安全。可以使用量模和量管元自由配置滴定,并在需要展一台螺旋拌器。在需要可以通相的件功能可平行滴定升 OMNIS Advanced Titrator。

- 通算机或本地网控制
- 可以其他用或助溶液外接四个滴定模或加液模
- 螺旋拌器的接方式
- 可提供不同大小的量管:5、10、20 或 50 mL
- 采用 3S 技的瓶配器:安全理化学品,自生商的原始数据

量模式和件:

- 点定滴定:“Basic” 功能可
- 点和等当点滴定(一/):“Advanced” 功能可
- 点和等当点滴定(一/),包括平行滴定:“Professional” 功能可



板 (0.15 x 8 x 8 mm) 的玻璃鞘,板化,用于化原滴定(双伏安滴定法)。特用于

- 生素 C 定
- 量的定
- 指数
- 葡萄酒中的硫酸 (SO_2)
- 按照温克勒法的含量