



Application Note AN-T-217

Hypochlorite and sodium chloride in disinfectant

Reliable all-in-one determination by argentometric titration

Disinfectants play an important role worldwide. Especially in times of widespread diseases, it is essential to protect humans and animals from harmful bacteria, viruses, or fungi. Animal diseases such as bird or swine flu or more communicable viruses like COVID-19 can cause billions in economic damage and even destroy entire industrial sectors.

Sodium hypochlorite and sodium chloride can be effectively used as disinfectants for water and for surfaces. They are widely available and inexpensive. However, it is essential to make the

correct dilution in order to achieve the most efficient disinfection. The World Health Organization (WHO) recommends (depending on the application) concentrations in disinfectants of 1000–5000 mg/L NaOCl and up to 200 g/L NaCl.

This Application Note demonstrates a reliable method to determine the hypochlorite and sodium chloride content in disinfectants by two subsequent argentometric titrations in the range recommended by the WHO.

SAMPLE AND SAMPLE PREPARATION

Two samples containing approximately 500 mg/L (Sample 1) and 5000 mg/L (Sample 2) sodium hypochlorite and approximately 200 g/L

EXPERIMENTAL

The analysis consists of two subsequent titrations with silver nitrate. In a first titration, the sodium hypochlorite content is determined by back-titration of an excess of potassium iodide. Immediately afterwards, the sodium chloride content is determined in the same sample.

The analysis is performed on a system consisting of an OMNIS Advanced Titrator and OMNIS Dosing Modules equipped with an Ag-Titrode. After transferring an appropriate amount of sample into the titration vessel, a sufficient amount of deionized water is added to immerse the electrode. Nitric acid and potassium iodide are added, and the titrations are carried out using standardized silver nitrate as titrant.

RESULTS

The analysis demonstrates acceptable results. The lower hypochlorite content and higher standard deviation are due to the instability of

sodium chloride in each are analyzed. No further sample preparation is required.

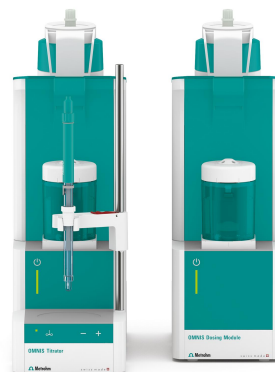


Figure 1. OMNIS Advanced Titrator and OMNIS Dosing Module equipped with Ag-Titrode for the determination of hypochlorite and sodium chloride content in disinfectant.

hypochlorite. It is therefore recommended to analyze the sample immediately after sampling. The results are displayed in **Table 1**.

Table 1. Results of the hypochlorite and sodium chloride determination in disinfectants (n = 6)

	Sample 1	Sample 2
Hypochlorite content in mg/L	460	4993
SD(rel) in %	7.4	1.1
Sodium chloride content in g/L	202.4	198.3
SD(rel) in %	0.3	0.7

CONCLUSION

Titration is a precise and reliable method to determine the hypochlorite and sodium chloride content in disinfectants.

Using an OMNIS Advanced Titrator equipped with an Ag-Titrode allows a fast all-in-one

determination. The OMNIS system offers the opportunity to customize the system according to your need and expand it for other required titration applications.

Internal reference: AW TI CH1-1308-052020

CONTACT

瑞士万通中国
北京市海淀区上地路1号院
1号楼7702
100085 北京

marketing@metrohm.com.cn

CONFIGURATION



OMNIS Titrator Salt

OMNIS Titrator Salt 提供了用于量滴定的完整套件。套件包含:配有磁力拌器的 OMNIS Advanced Titrator、一个 10 mL 的量管元、一个有硝酸的滴定用的 d-AgTitrode 以及 OMNIS 件的独立可。