



Application Note AN-V-070

Determination of iodide in glacial acetic acid

Iodide determination by cathodic stripping voltammetry (CSV) at the HMDE (hanging mercury drop electrode)

Methyl iodide is a key ingredient to facilitate chemical reactions during production of glacial acetic acid. However, this raises the chance of iodide ending up in the final product. This is a problem because manufacturers commonly use acetic acid as a reagent to produce other chemicals, such as vinyl acetate. Even trace amounts of iodide can poison the catalysts used in these processes, increasing costs, and negatively affecting product quality. Regular determination of the iodide concentration

ensures the desired quality of acetic acid, safeguarding the integrity of various downstream industrial processes.

Using ICP-MS to measure iodine in glacial acetic acid faces challenges due to memory effects that cause high background signals. Cathodic stripping voltammetry (CSV) at the hanging mercury drop electrode (HMDE) overcomes these limitations and provides a robust, cost-effective, and convenient alternative.

SAMPLE

Glacial acetic acid, 99.8%

EXPERIMENTAL

Add 10 mL acetic acid sample and then 2 mL ultrapure water into the measuring vessel. Carry out the determination of iodide using the 884 Professional VA (Figure 1) and the parameters specified in Table 1. The concentration is determined by two additions of iodide standard addition solution.



Figure 1. 884 Professional VA manual for MME.

Table 1. Parameters

Parameter	Setting
Mode	HMDE
Deposition potential	0.1 V
Deposition time	30 s
Start potential	-0.15 V
End potential	-0.5 V
Sweep rate	13 mV/s
Peak potential iodide	-0.32 V

ELECTRODES

- Multi-Mode Electrode pro

RESULTS

The method is suitable for the determination of iodide in acetic acid samples. The limit of detection of the method (for a deposition time of 30 s) is approximately 1 µg/L.

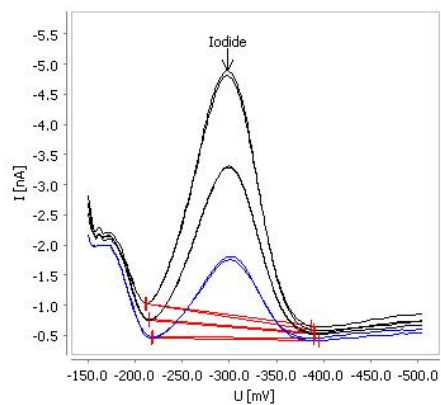


Figure 2. Determination of iodide in glacial acetic acid with CSV.

Table 2. Result

Sample	Iodide (µg/L)
Acetic acid	4.85

CONTACT

117702
100085

marketing@metrohm.com.c
n

CONFIGURATION



(MME) 884 Professional VA manual

用于多模式 (MME) 的 884 Professional VA manual 是借助多模式 pro 或 scTRACE Gold 或液滴使用伏安法和法行高端痕量分析的入器。此已的瑞士万通技与高效位/恒位以及外接的活 viva 件用,在重金属定域中展了新的前景。有的校准器的恒位在每次量之前均自冲洗行校准,保可能的最高精度。

通此器也可使用旋行定,例如借助«循伏安溶出法»(CVS)、«循脉冲伏安溶出法»(CPVS)和位法(CP)定池中的有机添加。借助可更的量,可在使用不同的各用之快速切。

使用 viva 件行控制、数据采集和估。

用于 MME(多模式)的 884 Professional VA manual 供配大量附件,包括用于多模式 pro 的量。和 viva 可独。