



Application Note AN-V-197

Indirect determination of iodide in brine with stripping voltammetry

Quantification of iodide in the chlor-alkali process through iodate formation with the hanging mercury drop electrode

Monitoring the iodide concentration in NaCl brine is crucial during membrane process-based chlor-alkali electrolysis. Iodide can easily oxidize to iodate during electrolysis, leading to its precipitation and fouling of the membrane surface. Fouling can reduce the high efficiency of

the membrane process and lead to increased energy consumption and decreased product quality. Therefore, monitoring the iodide concentration can help prevent fouling and protect the expensive membranes used in this process.

Stripping voltammetry, with its low detection limit and quick analysis capabilities, emerges as an attractive tool for the analysis of iodide in highly concentrated brines. By utilizing voltammetry, chlor-alkali plants can effectively

monitor and manage iodide levels, thus preventing membrane fouling. This approach not only preserves membrane durability and function but also results in high performance of the electrolysis process.

SAMPLE

Sodium chloride brine, β (NaCl) = 300 g/L

EXPERIMENTAL

Add 10 mL oxidized sodium chloride brine sample and 2 mL of ultrapure water into the measuring vessel. The determination of iodide is carried out with the 884 Professional VA (Figure 1) using the parameters specified in Table 1. The concentration is determined by two additions of iodate standard addition solution.



Figure 1. 884 Professional VA manual for MME.

Table 1. Parameters

Parameter	Setting
Mode	HMDE
Start potential	-0.7 V
End potential	-1.3 V
Sweep rate	13 mV/s
Peak potential iodide	-1.05 V

ELECTRODES

- Multi-Mode Electrode pro

RESULTS

The chlor-alkali brine solution contains a high concentration of chloride ions that can interfere with the direct measurement of iodide. By converting iodide to iodate, these interferences are minimized. The determined iodate concentration is then recalculated as iodide concentration as indicated in **Table 2**.

The method is suitable for the determination of low concentrations of iodide in sodium chloride brine (β (NaCl) = 300 g/L) samples.

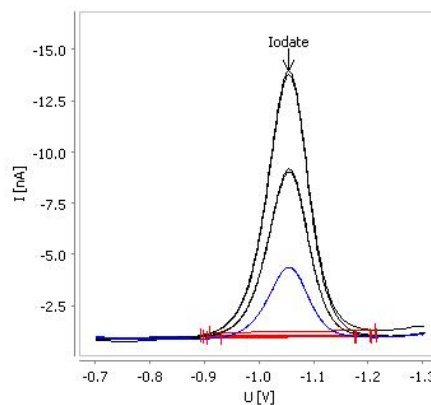


Figure 2. Determination of iodate in sodium chloride brine with stripping voltammetry.

Table 2. Result

Sample	Iodate ($\mu\text{g/L}$)
Sodium chloride brine	72.86

Table 2. Result

Sample	Iodate ($\mu\text{g/L}$)
Sodium chloride brine	72.86
Sample	Iodide ($\mu\text{g/L}$)
Sodium chloride brine	52.63

CONTACT

瑞士万通中国
北京市海淀区上地路1号院
1号楼7702
100085 北京

marketing@metrohm.com.cn

CONFIGURATION



(MME) 884 Professional VA manual

用于多模式 (MME) 的 884 Professional VA manual 是借助多模式 pro 或 scTRACE Gold 或液滴使用伏安法和法行高端痕量分析的入器。此已的瑞士万通技与高效位/恒位以及外接的活 viva 件用,在重金属定域中展了新的前景。有的校准器的恒位在每次量之前均自冲洗行校准,保可能的最高精度。

通此器也可使用旋行定,例如借助«循伏安溶出法»(CVS)、«循脉冲伏安溶出法»(CPVS)和位法(CP)定池中的有机添加。借助可更的量,可在使用不同的各用之快速切。

使用 viva 件行控制、数据采集和估。

用于 MME(多模式)的 884 Professional VA manual 供配大量附件,包括用于多模式 pro 的量。和 viva 可独。